



THURLBY THANDAR INSTRUMENTS

PSA1301T *1.3GHz PORTABLE SPECTRUM ANALYZER*

INSTRUCTION MANUAL

Table of Contents

1. Supplied Items	5
2. Using This Manual & Meaning of Terms	5
3. Warranty and Support	6
4. Initial Operations	6
4.1. Charging the Batteries	6
4.2. Initialising the Palm T X	6
4.3. Software provided by Palm on CD	6
4.4. Linking to a Personal Computer	6
5. First Use of the Spectrum Analyzer	7
5.1. Quick Start Guide	7
5.2. Detailed Operating Guide	7
6. Product Description and Capabilities	8
7. Specification	9
7.1. Frequency Measurement	9
7.2. Amplitude Measurement	9
7.3. Sweep	10
7.4. Signal Input	10
7.5. Demodulation (Zero Span mode)	10
7.6. Display	11
7.7. Memory Storage	11
7.8. Connectors	11
7.9. Power Sources	12
7.10. Mechanical	12
7.11. Environmental and Safety	12
8. Declaration of Conformity	13
9. EMC	14
10. Safety	15
11. Connections	16
11.1. RF Signal Input	16
11.2. DC Power Input	16
11.3. Demodulated Audio Output	16
11.4. USB 'through' Connector	16
12. Stylus	17
13. Memory Card	17
13.1. Removing and Inserting the Card	17
13.2. Using an Alternative Card	17
13.3. Card Storage Capacity	18
14. Removing and Re-fitting the Palm T X	18

15. Re-initialising the Palm T X	19
15.1. Procedure for Re-Initialising	19
15.2. Technical Note about the OFF state	19
16. Language Choice for the Palm T X	19
17. Turning On and Turning Off	20
17.1. Palm T X On/Off	20
17.2. PSA1301 On/Off Control	20
17.3. Operation Delay after Turning On	20
18. Battery and AC Power	21
18.1. Battery Operation	21
18.2. AC Power Operation	21
18.3. Extended Periods Without Use	22
19. Using the PSAnalyzer Application	22
19.1. Initial Conditions	22
19.2. Selecting and Leaving the Application	22
19.3. Touch Screen or Hard Key operation	22
19.4. The PSAnalyzer Screen	23
19.5. Operation and Navigation	23
19.6. Turning Off / Power Saving	24
20. The PSAnalyzer Menu System	24
20.1. Home Menu	24
20.2. Menus Summary	24
20.3. Mode Menu	25
20.4. Centre Menu	25
20.5. Step Value Sub Menu	26
20.6. Span Menu	26
20.7. Start Frequency Menu	27
20.8. Stop Frequency Menu	27
20.9. AM/FM Menu	27
20.10. Level Menu	28
20.11. Markers Menu	28
20.12. Sweep Menu	29
20.13. Traces Menu	29
20.14. Stores Menu	30
20.15. System Menu	31
20.16. Exit Menu	31
21. PSAnalyzer Operating Techniques	32
21.1. Menu Navigation	32
21.2. Frequency Setting	32
21.2.1. Centre/Span and Start/Stop modes	32
21.2.2. Centre Menu Shortcuts	32

21.2.3.	Span Menu Shortcuts	32
21.2.4.	Start and Stop Menu Shortcuts	32
21.2.5.	Setting by Direct Numeric Entry	33
21.2.6.	Setting by Tab and Jog	33
21.3.	Performing Sweeps	33
21.4.	Level Measurements	34
21.5.	The PRESET Key	34
21.6.	Using Markers	34
21.7.	Reference Trace	35
21.8.	Store, Recall and Copy	35
21.9.	Screen Resolution and Trace Thickness	36
21.10.	Changing the Palm Input Area type	36
21.11.	Adjusting the Display Brightness	36
22.	Help Screens	36
23.	Functions outside of PSAnalyzer	37
23.1.	Viewing a Stored Screen Image	37
23.1.1.	Adding Annotation to Screens	37
23.2.	Printing a Stored Screen Image (using a printer connected to a PC)	37
23.3.	Transferring PSAnalyzer Files to a Personal Computer	37
23.3.1.	Using the Memory Card Reader	38
23.4.	Sending PSAnalyzer Files via Bluetooth or WiFi	38
23.4.1.	Email Attachments	38
23.4.2.	Sending Images from the Media application	38
23.4.3.	Direct File Transfer using WiFile LT	38
24.	PSAnalyzer Files and Defaults	39
24.1.	Factory Default Settings for PSAnalyzer	39
24.2.	File Locations for PSAnalyzer data files	39
24.3.	File Structures for PSAnalyzer data files	39
25.	Maintenance, Calibration and Repair	40
25.1.	Screen Protection	40
25.2.	Cleaning	40
25.3.	Maintaining Battery Condition	40
25.4.	Calibration	40
25.5.	Service & Repair	40
26.	Trouble Shooting	41
26.1.	Correcting Unexpected Conditions in PSAnalyzer	41
26.2.	Resetting the Palm T X	41
26.3.	Reinstalling or Updating the PSAnalyzer application	42
26.4.	Card Reader Installation Problems	42

27. Support Information and Accessories	43
27.1. Support Information for the Palm T X	43
27.2. Standard Accessories supplied for the Palm T X	43
27.3. Optional Accessories	43
28. Appendix A. Using other functions of the Palm T X	44
28.1. Handhelds and PDAs - Overview	44
28.2. Software provided by Palm on CD	44
28.3. Linking to a Personal Computer	44
28.3.1. USB connections to a PC	45
28.4. Palm Desktop software	45
28.5. Core Capabilities of the Palm T X	45
28.6. Standard Applications	46
28.7. Additional Applications	47
28.8. Some Palm Basics	47
28.8.1. Operating System, Memory and Filing System	47
28.8.2. Modes of Operation	47
28.8.3. Hard Keys	48
28.8.4. Task Bar	48
28.8.5. Application Help	48
28.8.6. Menu Options	49
28.8.7. Categories	49
28.8.8. Files and Folders on the Memory Card	49
28.8.9. Communicating with Other Devices	50
28.9. HotSync	50
28.10. Creating a Shortcut to PSAnalyzer	51
28.11. Additional Software Applications	51
28.11.1. Installing additional applications without using Palm Desktop	52
29. Appendix B. Palm Desktop Software	53
29.1. Deciding whether to install Palm Desktop	53
29.2. The purpose of Palm Desktop software	53
29.3. HotSync	53
29.4. Palm T X User Name	53
29.5. Palm Desktop software and Windows PCs	54
29.6. Palm Desktop software and Apple Macintosh computers	54
29.7. Installation Procedure	54
29.8. Using multiple devices with one PC, or a device with multiple PCs	55
29.9. HotSync transfer of PSAnalyzer Screen Images to a PC	55

1. Supplied Items

The PSA1301T portable spectrum analyzer is made up of four main items:

- The PSA1301 spectrum analyzer unit manufactured by TTI.
- The Palm T|X handheld computer manufactured by Palm, Inc.
- The PSAnalyzer software application created by TTI to run on the Palm T|X.
- An SD (or MMC) Memory Card for storing and transferring data

The following support items are also provided by TTI:

- “Read This First” leaflet.
- Universal mains adaptor/charger.
- USB lead (mini B plug to standard A plug).
- SD/MMC USB Card Reader (with USB extension lead where necessary).
- Printed instruction manual (English only).
- Support CD containing multi-language manual and backup software.
- M2.5 security screws to prevent easy removal of the Palm T|X (if required).
- Transparent storage case for memory card.

The PSA1301T is supplied with the Palm T|X mounted into the PSA1301, and the PSAnalyzer software application pre-installed. The memory card is fitted into the Palm T|X.

All of the software and accessories provided by Palm for the T|X are contained within the Palm T|X shipping box.

Note: The SD/MMC USB Card Reader and other small items may be packed inside the Palm T|X shipping box.

2. Using This Manual & Meaning of Terms

Cross References within this Manual

This manual is also provided as multi-language PDF files. The manual includes many cross references which are shown as follows - see section [X.X](#).

Within a PDF file, the boxed number is a hyperlink to that section number, thus enabling the user to jump rapidly the section referred to and then jump back to continue reading the text.

TTi

TTi is used throughout this manual as the abbreviation for Thurlby Thandar Instruments Ltd.

Palm and palmOne

The Palm T|X is manufactured by Palm, Inc. The company was until recently using the name palmOne, but has now reverted to its original name of Palm. Hardware and support software items may be branded either Palm or palmOne. The name Palm is used throughout this manual, but may refer to items branded palmOne. Palm and palmOne are registered trademarks of Palm, Inc.

Handheld Computer and PDA

Devices such as the Palm T|X are commonly described as handheld computers, palmtop computers or PDAs (personal digital assistants). The term ‘handheld computer’ is used throughout this manual.

PSA1301

This is used to describe the spectrum analyzer unit excluding the Palm T|X handheld computer.

PSA1301T

This is used to describe the complete spectrum analyzer unit including the Palm T|X handheld computer.

3. Warranty and Support

The warranty for the PSA1301 spectrum analyzer unit is provided by TTI. The warranty for the Palm T|X handheld computer is provided by Palm - details of the warranty are contained within the Palm T|X shipping box or on the Palm website.

TTi (or its agents and distributors) will provide technical support for the PSA1301T spectrum analyzer based around use of the PSAnalyzer software application.

TTi (or its agents and distributors) will NOT provide technical support for any other functions of the Palm T|X outside of the PSAnalyzer software application. Technical support for all other functions must be obtained from Palm or from associated support websites. **See section 27.1.**

4. Initial Operations

4.1. Charging the Batteries

It is probable that the batteries will be discharged when the product is received. Consequently the first action should be to charge the unit using the supplied mains adaptor. To fully charge the batteries it should be left charging for 4 hours.

4.2. Initialising the Palm T|X

If the battery has been fully discharged, the Palm T|X handheld computer will have to be re-initialised before the spectrum analyzer can be used. **Details of how to re-initialise it are given in section 15.**

Note: The PSA1301 spectrum analyzer adaptor does not require any manual initialisation.

4.3. Software provided by Palm on CD

The software and support information provided by Palm assumes that you will want to link your Palm T|X to a personal computer on a regular basis. The Palm "Read this First" manual instructs you to load the CD software immediately as part of the initial set up.

Users of the PSA1301T do not need to do this unless they choose to. TTI recommends that users read the relevant sections of the Palm documentation and consider their own use of the product before deciding whether to install to Palm software. **Also read Appendix B, section 29 of this manual.**

! Note: Do **NOT** make a USB connection between the PSA1301T (or the Palm T|X) and a PC unless the Palm software has already been installed.

4.4. Linking to a Personal Computer

It is NOT necessary ever to link the PSA1301T to a personal computer. It is a self contained instrument which can perform its primary function of RF spectrum analysis without linkage to other devices. TTI provides a USB linked memory card reader in order that PSAnalyzer files can be transferred to a PC where this is required.

However some of the additional features of the Palm T|X do require linking to a personal computer in order to share information, load new software applications and transfer files.

See section 28.3 for information on this subject.

5. First Use of the Spectrum Analyzer

After charging the battery and initialising the Palm T|X, it will then be possible to use the Spectrum Analyzer by launching the PSAnalyzer application.

! TTI recommends that you should read this manual in full before using the PSA1301T.

However, if immediate use of the spectrum analyzer is required, the following procedure can be used to start making measurements quickly.

5.1. Quick Start Guide

! **Before commencing** - the batteries must have been charged and the Palm T|X initialised as described in sections [4.1](#) and [15](#) respectively.

1. Connect signal to be measured - connect signal to the SMA connector at the top of the PSA1301.



The maximum allowable signal without damage is +20dBm (2.2 V rms). The maximum measurable signal is 0dBm (223 mV rms). If there is a possibility of the signal exceeding these levels, add suitable in-line attenuation.

2. Launch PSAnalyzer application - enter the Applications screen (by pressing the Home key once or twice). Press the PSAnalyzer icon on the touch screen of the Palm T|X, or select it by pressing the centre button of the 5-way navigator twice.



PSAnalyzer (The touch screen can be operated with a finger tip or the stylus of the Palm T|X)

3. Select Mode Menu - use the 5-way navigator to highlight and then select the Mode key, or press the key directly.



4. Select Preset - select using the 5-way navigator or press the key directly.



This sets maximum span (0.15MHz to 1300MHz), attenuation on, 280kHz bandwidth, sweep mode normal, setting mode Start + Stop, Markers M1 & M2 On.

5. Observe the Sweep - the sweep time will be circa 10 seconds (slow because of the wide span).

6. Set Markers - select the markers function, then use the 5-way navigator to move the markers to either side of the area of interest.

7. Set sweep width to markers - exit Markers (by pressing the Back hard key) and select the Start menu. Select Start=M1/Stop=M2 - the start and stop frequencies for the sweep are set to the marker points.

The above procedure should be sufficient to get started. Thereafter adjustments can be made to sweep parameters, attenuator, resolution bandwidth, etc. as may be appropriate to the signals being observed.

Basic on-screen help information for every menu is available by pressing the Help hard key. Some general information regarding the capabilities of the unit is available from the Info key on the Exit menu.

5.2. Detailed Operating Guide

To fully understand the operation of the PSA1301T and PSAnalyzer, it is necessary to read this manual.

From an operating point of view, the key sections are "Using the PSAnalyzer Application" section [19](#), "The PSAnalyzer Menu System" section [20](#), and "PSAnalyzer Operating Techniques" section [21](#).

6. Product Description and Capabilities

Brief Summary

The PSA1301T is a fully portable spectrum analyzer incorporating a handheld computer (a Palm T1X). It is sufficiently small and lightweight to be operated as a handheld instrument and has a typical battery life of four hours from each charge. Alternatively it can be used as a bench instrument using the supplied mains adaptor/charger. It can be set horizontally or vertically, or at an angle of about 25 degrees using its built-in tilt stand.

The spectrum analyzer has a frequency range of 0.15 MHz to 1300 MHz. The span can be set anywhere between 0.320 MHz and 1299.850 MHz with a resolution of 1kHz. Start, stop or centre frequencies can be set to the same resolution. The resolution bandwidth is selectable as 280 kHz or 15 kHz.

The on-screen amplitude range is 80 dB with a reference level of -20dBm or 0dBm. Vertical magnification to 5dB/div can be selected. Average noise floor is better than -90dBm at -20dBm reference level and 15 kHz RBW.

Sweeps can be continuous, single shot, peak hold or average (2 to 256 sweeps). Sweep time is defined by the span and resolution bandwidth, and varies between 0.1 sec and 30 sec. A zero span mode is available with AM or FM audio demodulation.

Twin vertical marker lines are available giving a readout of frequency and amplitude to resolution of 0.1 kHz and 0.1 dB. Markers can be manually positioned or automatically peak finding and tracking.

A reference trace can be displayed in addition to the live trace. The graticule is fully controllable. Any number of traces can be stored to permanent memory for recall to the screen or for data export. Instrument set-ups and complete screen bitmaps can also be stored.

Battery life depends upon screen brightness, but is around four hours of continuous operation from a charge. To conserve the battery, auto-sleep mode can be selected whereby the unit turns off automatically after a defined period from the last key press. All data is retained when off.

Pressing the Help hard key brings up a help screen relevant to the current menu position.

Full details of the product capabilities are given with the Specification section [7](#) and Using the PSAnalyzer Application section [19](#) onwards.

7. Specification

7.1. Frequency Measurement

Frequency Span

Frequency Range:	150 kHz to 1300 MHz (in one range)
Setting Modes:	Centre frequency plus Span, or Start frequency plus Stop frequency
Maximum Span:	1299.85 MHz (150 kHz to 1300 MHz)
Minimum Span:	320 kHz, or Zero Span with demodulation
Setting Resolution:	1 kHz at any frequency
Setting Accuracy:	Reference Frequency Accuracy for Start, Stop & Centre (Zero-Span) frequencies

Reference Frequency Accuracy

Initial Accuracy:	Better than ± 10 ppm at 20°C
Stability:	Better than ± 10 ppm over 10°C to 30°C
Ageing:	Better than ± 3 ppm per year

Phase Noise

Phase Noise:	Typically -100dBc/Hz at 100kHz offset at 500MHz
--------------	---

Resolution Bandwidth

RBW:	Selectable as 280 kHz or 15 kHz
Video Filtering:	Selectable independently of RBW setting

Frequency Markers

Number of Markers:	One, Two, or None
Marker Resolution:	0.1 kHz at all frequencies
Marker Accuracy:	$1/320^{\text{th}}$ of Frequency Span ± 0.1 kHz + Reference Frequency Accuracy
Frequency Readout:	The frequencies at the marker points and frequency difference are displayed simultaneously

7.2. Amplitude Measurement

Amplitude Range

Display Range:	80 dB
Reference Level:	Selectable as -20 dBm or 0dBm

Amplitude Accuracy

Ref. Level Accuracy:	Better than ± 1 dB at 50MHz at 10dB below reference level (20°C \pm 5°C)
Level Flatness:	Better than ± 1.5 dB relative to 50MHz over 500kHz to 1300MHz
Amplitude Linearity:	Better than ± 1 dB over 50dB range down from reference level

Noise Floor

Noise Floor: Better than -90 dBm average displayed noise floor
(reference level = -20 dBm, RBW = 15 kHz)

Distortion and Spurii

3rd Order Intermod.: < -60dBc for two signals at 10dB below reference level (500MHz and 501MHz)

Harmonic: < -60dBc at 10dB below reference level (100MHz)

1st & 2nd Image: <- 55dBc, typically <- 60dBc

Residual Spurii: Below noise floor

Amplitude Markers

Number of Markers: One, Two, or None

Marker Resolution: 0.1 dB

Amplitude Readout: The level at the marker points and level difference are displayed simultaneously

7.3. Sweep

Sweep Method: Peak detection for 320 points per sweep. The amplitude of the peak level found within each sub-span is stored (sub-span = span/320).

Sweep Time: Set automatically by Span and RBW.
Typically 200ms + 8ms/MHz of span (RBW = 280kHz)
Typically 200ms + 80ms/MHz of span (RBW = 15kHz)

Sweep Modes: Normal (continuous), Single, Peak Hold, or Average (2 to 256 sweeps)

Sweep Control: Separate buttons for Run and Stop. Peak Hold and Average are reset whenever Run is pressed.

7.4. Signal Input

Input Connector: SMA connector, 50 Ohms

VSWR: 1.5:1 typical



Absolute
Maximum
Input Level: + 20 dBm (2.2V rms) or 15V dc

7.5. Demodulation (Zero Span mode)

Demod. Modes: AM or FM

Display: Carrier amplitude only (horizontal line).

Audio Out: 30 mW into 32 Ohms mono or stereo headphones, adjustable volume, 3.5mm jack socket

7.6. Display

Display Type:	3.7 inch (9.4 cm) transfective backlit TFT LCD, 480 x 320 pixels total, 16 bit colour, touch screen.
Trace Area:	300 x 320 pixels (high resolution mode).
Graticule:	8 x 10 divisions light grey graticule. Selectable as fully on, horizontal lines only, or off).
Displayed Points:	320 points per sweep (peak detected).
Live Trace:	Dot-joined trace from current or held sweep. Selectable on or off.
Reference Trace:	Stored trace either recalled from memory or copied directly from live trace. Selectable on or off.
Resolution Modes:	Selectable as High Resolution or Low Resolution *

* In low resolution mode the trace area becomes 150 x 160 points where each point is a block of 4 pixels. Only 160 sweep points are displayed. This mode is useful in situations where the display could otherwise be difficult to see - e.g. when the instrument cannot be viewed at an optimum distance.

7.7. Memory Storage

Memory Type:	Non volatile Flash memory using removable SD or MMC memory cards.
Store Trace:	Any number of traces can be stored under either default file names or user entered file names. Traces are stored as tables of amplitude versus frequency and can be imported into other programs, as well as being recalled to the screen.
Recall Trace:	Recalls any stored trace to the reference trace of the display.
Store Set-up:	Any number of instrument set-ups can be stored under either default file names or user entered file names. All settings of the instrument are saved.
Recall Set-up:	Recalls any stored set-up, overwriting the existing settings of the instrument.
Store Screen:	This function copies the whole screen area to memory as a bit-map. Any number of screens can be stored under either default file names or user entered file names. Screen bit-maps can be viewed using the "Media" application of the Palm T X, or transferred to a PC for printing.

7.8. Connectors

RF Input Connector:	Standard SMA connector.
Power Connector:	1.3 mm dc power socket (centre positive) for 5.2V/1A external AC power adaptor/charger as supplied by TTI.
USB Connector:	Mini USB connector (5 pin mini B) which provides direct access to the USB port of the Palm T X.
Audio Connector:	3.5 mm jack socket for demodulated audio out (accepts mono or stereo plugs).

7.9. Power Sources

AC Line Operation/Charging

The PSA1301T can be operated from mains power using the AC power adaptor provided by TTI. This powers and recharges both the PSA1301 Spectrum Analyzer and the Palm T|X simultaneously.

AC Adaptor/Charger

Input Voltage Range: 100V to 240V nominal 50Hz/60Hz. Interchangeable plus for UK, Euro, USA and Australia are supplied.

Battery Operation

The PSA1301 and the Palm T|X contain their own internal rechargeable battery packs. The PSA1301 is turned off automatically whenever the PAnalyzer program is exited, or when the Palm T|X is turned off.

PSA1301 Spectrum Analyzer

Battery Type: Ni-Mh 3.6V 700mA-hr (3 x AAA cell)

Battery Life: > 5 hours continuous operation

Recharge Time: < 3 hours from fully discharged

Palm T|X

Battery Type: Li-ion 3V 1050mA-hr

Battery Life: Typically 4 hours continuous operation (depending on backlight brightness)

Recharge Time: < 4 hours from fully discharged

Auto Sleep Mode

To conserve battery life, the system can be set to automatically switch into sleep mode after a defined time from the last key press. This can be set between 5 mins and 60 mins (or never).

7.10. Mechanical

Size: 170mm high x 97mm wide x 47mm deep (including feet)

Weight: 495 grms total including Palm T|X.

Tilt Stand: Built-in tilt stand for bench use which angles the unit at approximately 25 degrees to the horizontal and can alternatively be used as a hook mount.

7.11. Environmental and Safety

Operating Range: +5°C to + 40°C, 20% to 80% RH.

Storage Range: -10°C to +50°C

Environmental: Indoor use at altitudes to 2000m, Pollution Degree 2.

Electrical Safety: Complies with EN61010-1.

EMC: Complies with EN61326.

8. Declaration of Conformity

EC Declaration of Conformity

We Thurlby Thandar Instruments Ltd
Glebe Road
Huntingdon
Cambridgeshire PE29 7DR
England

declare that the

PSA1301T 1.3GHz Spectrum Analyzer

meets the intent of the EMC Directive 89/336/EEC and the Low Voltage Directive 73/23/EEC. Compliance was demonstrated by conformance to the following specifications which have been listed in the Official Journal of the European Communities.

EMC

Emissions: a) EN61326 (1998) Radiated, Class B

Immunity: EN61326 (1998) Immunity Table 1, Performance B, referring to:

- a) EN61000-4-2 (1995) Electrostatic Discharge
- b) EN61000-4-3 (1997) Electromagnetic Field
- c) EN61000-4-4 (1995) Fast Transient

Safety

EN61010-1 Pollution Degree 2.



CHRIS WILDING
TECHNICAL DIRECTOR
2 January 2006

Spectrum Analyzer

This instrument has been designed to meet the requirements of the EMC Directive 89/336/EEC. Compliance was demonstrated by meeting the test limits of the following standards:

Emissions

EN61326 (1998) EMC product standard for Electrical Equipment for Measurement, Control and Laboratory Use. Test limits used were:

- a) Radiated: Class B

Immunity

EN61326 (1998) EMC product standard for Electrical Equipment for Measurement, Control and Laboratory Use.

Test methods, limits and performance achieved were:

- a) EN61000-4-2 (1995) Electrostatic Discharge : 4kV air, 4kV contact, Performance A.
- b) EN61000-4-3 (1997) Electromagnetic Field, 3V/m, 80% AM at 1kHz, Performance B.
- c) EN61000-4-4 (1995) Fast Transient, 0.5kV peak (signal input), Performance B.

Adaptor/Charger

This AC adaptor/charger has been designed to meet the requirements of the EMC Directive 89/336/EEC.

Compliance was demonstrated by meeting the test limits of the following standards:

Emissions

EN55022, radiated and conducted Class B.

Immunity

Test methods, limits and performance achieved were:

- a) EN61000-4-2 (1995) Electrostatic Discharge : 4kV air, 4kV contact, Performance B.
- b) EN61000-4-3 (1997) Electromagnetic Field, 3V/m, 80% AM at 1kHz, Performance A.
- c) EN61000-4-11 (1994) Voltage Interrupt, 30% reduction, 10ms, Performance B; 60% reduction 100ms, Performance C.
- d) EN61000-4-4 (1995) Fast Transient, 1kV peak (AC line), Performance B
- e) EN61000-4-5 (1995) Surge, 1kV (line to line), 2kV (line to ground), Performance B.
- f) EN61000-4-6 (1996) Conducted RF, 3V, 80% AM at 1kHz (AC line only; DC Output connection <3m, therefore not tested), Performance A.

Performance Definitions

The definitions of performance criteria are:

Performance criterion A: 'During test normal performance within the specification limits.'

Performance criterion B: 'During test, temporary degradation, or loss of function or performance which is self-recovering'.

Performance criterion C: 'During test, temporary degradation, or loss of function or performance which requires operator intervention or system reset occurs.'

10. Safety

Spectrum Analyzer

This instrument is Safety Class III according to IEC classification and has been designed to meet the requirements of EN61010-1 (Safety Requirements for Electrical Equipment for Measurement, Control and Laboratory Use).

This instrument has been tested in accordance with EN61010-1 and has been supplied in a safe condition. This instruction manual contains some information and warnings which have to be followed by the user to ensure safe operation and to retain the instrument in a safe condition.

This instrument has been designed for indoor use in a Pollution Degree 2 environment in the temperature range 5°C to 40°C, 20% - 80% RH (non-condensing). It may occasionally be subjected to temperatures between +5° and -10°C without degradation of its safety. Do not operate while condensation is present.

Use of this instrument in a manner not specified by these instructions may impair the safety protection provided.

WARNING!

All accessible parts will be at the same voltage as the outer body of the SMA input socket. In particular, note that the shell of the mini-USB connector is galvanically connected to the body of the SMA input which will therefore be at earth ground potential when the USB port is connected to a desktop PC. To maintain user safety under all other circumstances it is essential that the input is not connected to a voltage above 30Vdc or 30Vrms with respect to earth ground which is the limit of Safe Extra Low Voltage (SELV) by IEC definition.

The instrument shall be disconnected from all voltage sources before it is opened for any adjustment, replacement, maintenance or repair.

Any adjustment, maintenance and repair of the opened instrument under voltage shall be avoided as far as possible and, if inevitable, shall be carried out only by a skilled person who is aware of the hazard involved.

Do not wet the instrument when cleaning it.

The following symbols are used on the instrument and in this manual.

 Direct Current



CAUTION – refer to accompanying documentation.

Damage to the instrument may occur if these precautions are ignored.

Adaptor/Charger

The adaptor/charger supplied has a universal input voltage rating of 100-240VAC, 50/60Hz. It is a Class II (double insulated) device, fully approved to EN 60950-1 (2001), UL 60950 (UL listing E138754) and AS/NZS CISPR:2002 (C-Tick).

11. Connections

11.1. RF Signal Input

The signal to be measured is connected via a standard (non reverse) SMA connector mounted at the top of the instrument. The input impedance is 50 Ohms. The maximum allowable input is +20dBm of RF power (approximately 2.2 volts RMS), or 15V DC.



Applying a signal above these levels could damage the unit and such damage would not be covered by the product warranty.

It should be noted that SMA connectors have a limited mechanical life and that, where frequent connection and disconnection is expected, a sacrificial intermediate connector should be used.

11.2. DC Power Input

DC power to operate and/or recharge the instrument is connected via a 1.3mm power socket mounted on the side of the instrument.



Use ONLY the mains adaptor provided by TTI with the unit. Use of any other power source will void the warranty.

The batteries of the spectrum analyzer unit and of the Palm T|X are automatically charged whenever dc power is connected.

An LED adjacent to the socket shows that the batteries of the PSA1301 are recharging. When they are fully charged this LED will go off. The charging state and charge level of the Palm T|X batteries is shown on the display of the T|X, see section [18.1](#).

11.3. Demodulated Audio Output

Demodulated audio (when in Zero Span Mode) is provided via a 3.5mm stereo jack socket mounted at the top of the instrument. Maximum power output is 32 milliwatts into 32 Ohms with the volume level adjustable from within the application.

The signal is mono but connection can be made using either a mono or stereo plug. In the latter case the signal will be present on both channels.

11.4. USB 'through' Connector

The USB port of the Palm T|X can be accessed via a mini USB connector (mini type B) mounted on the side of the instrument. A cable is provided to connect this to a standard computer USB port.

Note that the USB interface has no function within the PSAnalyzer application, the cable is supplied in order that Palm Desktop software can be used with the Palm T|X in situ within the PSA1301T.

Note: The USB cable should be disconnected at the PSA1301T end when using the PSAnalyzer application.

- ! **Important** - Do NOT try to make a USB connection to a PC which has not had the appropriate software loaded onto it. See section [28.2](#).

12. Stylus

Handheld computers such as the Palm T|X are normally operated using the supplied stylus. The PSAnalyzer application has been written so that use of a stylus is not a requirement, see section [19.2](#). Nevertheless some users may prefer to operate it using a stylus.

The stylus provided with the Palm T|X clips into a slot on its right hand edge. When the T|X is fitted into the PSA1301, the stylus fits into the same slot but is prevented from sliding as far down as normal by a stop incorporated within the top cover. This ensures that the stylus remains easily accessible.

Note: If access to the stylus is not required, it can be pushed past the stop. If this is done, however, it will not be possible to access it without removing the Palm T|X from the PSA1301T.

13. Memory Card

The PSA1301T is supplied complete with a Flash memory card (type SD or MMC). This card is necessary for storing and recalling traces, screens and set-ups in PSAnalyzer. A backup of the original PSAnalyzer program is also stored on the card.

The memory card can be used in many other Palm applications, both as additional memory and as a convenient way of sharing data with other devices. Note: Palm documentation refers to a memory card as an expansion card.

PSAnalyzer can be used without any card in place, but storing or recall of traces, screens or set-ups will not be available.

The memory card can be used as a means of transferring data to and from a PC using the USB card reader supplied. See section [23.3](#) for details.

13.1. Removing and Inserting the Card

The card fits into a slot on the top left hand edge of the Palm T|X and is slightly recessed relative to the top edge of the PSA1301.

To remove the card, press it down and then release it (a confirmation tone may be heard). The card becomes free and can be slid out. To insert the card, slide it into the slot and press it down firmly until a click is felt and the confirmation tone is heard.

Note: When a card is inserted, the Applications screen is automatically switched to show the applications which are on the card. In the case of the card supplied with the PSA1301T this will be the utility PSAInstaller. To return to the normal Applications screen, select the drop down menu at the top right and select "All" in place of "Card".

13.2. Using an Alternative Card

Any SD (secure digital) or MMC (multi media) card that is compatible with the Palm T|X can be used in place of the one supplied. When PSAnalyzer stores a file it automatically creates the required folder structure. Multiple cards could be used increase total capacity or to separate files related to different projects.

Note: The original card should be retained as it contains an important utility and a backup of the PSAnalyzer application. This card is labelled with the TTI logo and with the version number of the supplied PSAnalyzer software.

13.3. Card Storage Capacity

The size of the memory card supplied by TTI may vary from time to time, but will be in the range 32MB to 128MB.


The size of the files stored by PSAnalyzer are very small in comparison. Set-up files are a few hundred bytes each, trace files are around six kilobytes each, and screen bitmap files are 120 kilobytes each. Note, however, that the FAT16 format of the card creates a minimum file allocation size of 16 kilobytes (or possibly greater) for any file stored.

As a rough guide, a 64MB card can store 450 traces, 450 set-ups and 450 screens simultaneously, while a 128MB card would be able to store over 1,000 of each.

14. Removing and Re-fitting the Palm T|X

All of the functionality of the Palm T|X is available when it is mounted within the PSA1301 spectrum analyzer. However, users may wish to remove it in order to carry it in their pocket as a personal organiser or to use for other purposes. Removing and re-fitting is quick and simple.

Removing

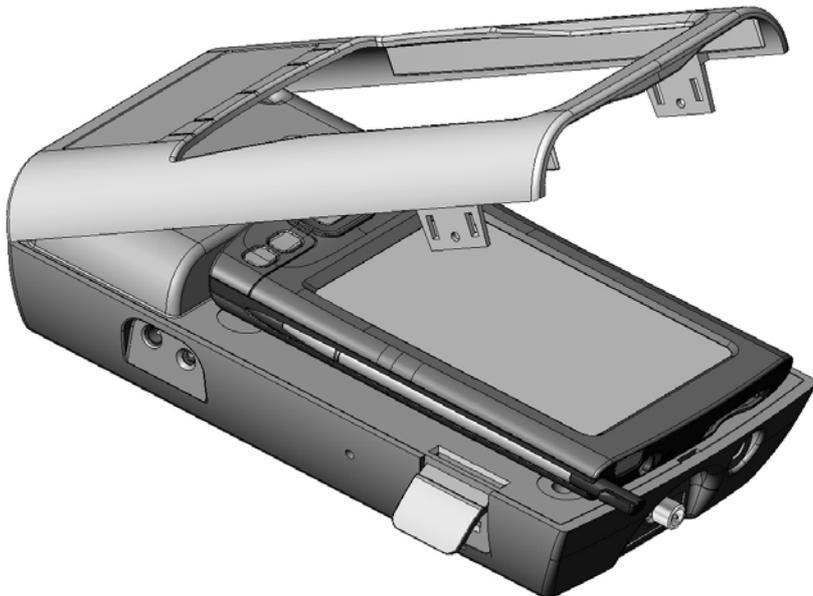

Lift the two latches close to the top of the unit and remove the silver top cover (see drawing). Remove the Palm T|X by gripping its sides and pulling it towards the top edge of the spectrum analyzer. (Note that the connector is a tight fit and that a hard pull may be needed).

Note: the top cover could be secured by screws under the latches which must be removed first (see section Preventing Unauthorised Removal below).

Re-fitting

Remove the Stylus from the Palm T|X. Push the Palm T|X onto the connector by pushing it firmly in the line of the instrument.

Ensure that the two fixing latches are open. Locate the top cover onto the rear of the instrument and lower it down, then operate the two fixing latches to secure it. Refit the Stylus.

Preventing Unauthorised Removal

In circumstances where removal of the Palm T|X is regarded as undesirable, the top cover can be secured using screws which fit underneath the two latches. TTI provides Torx head screws for this purpose (M2.5 size) although they are not fitted.

15. Re-initialising the Palm T|X

Whenever the battery of the Palm T|X has been allowed to completely discharge (as is normally the case when it is first received) it will be necessary to re-initialise it.

15.1. Procedure for Re-Initialising

Charge the Palm T|X in the normal way. After a short period (normally less than 10 minutes) the battery voltage will recover to a point where normal operation is possible. The T|X may then switch itself on automatically, or it may be necessary to turn it on manually (using the green button on the top edge).

At this point a Palm logo will appear on the screen and the unit will reboot (i.e. the operating system will reload) as indicated by moving black bars on the screen. When this is complete the user will be prompted to confirm or re-enter the real-time clock information (date, time, location) and confirm user preferences.

When this has been completed the Palm T|X is ready for use, however it should be left charging for several more hours before disconnecting it from the ac power adaptor/charger.

In exceptional circumstances, the Palm T|X may fail to re-initialise after being re-charged. Should this happen it will be necessary to operate the "Reset" button on the back of the T|X. To do this, remove the T|X from the PSA1301 (see "Removing and Re-fitting the Palm T|X" above), and use the Palm stylus to press the reset button, see section [26.2](#). It should then re-initialise.

15.2. Technical Note about the OFF state

Handheld computers operate on the principle of being 'always on'. When they are turned 'off', they merely go into a low power consumption mode with the display and other functions disabled - this is often referred to as Sleep mode. When turned back on, they restart instantly without the delay that would be caused if the operating system had to be reloaded.

Consequently when 'off', a small amount of power is still being taken from the battery. It is assumed that the user will keep the unit charged and never let the battery fully discharge.

In most handheld computers, allowing the battery to fully discharge would cause all of the user's data to be lost. However, the Palm T|X uses permanent Flash memory which prevents user data from being lost if the battery is fully discharged. The real-time clock, however, cannot continue to run with a fully discharged battery.

If the unit is left unused and unconnected to its charger for an extended period (typically several weeks) the battery will discharge to a point where re-initialisation is needed.

The batteries of the PSA1301 will also discharge over an extended period of time, but no re-initialisation should be required.

16. Language Choice for the Palm T|X

As supplied with the PSA1301T, the operating language of the Palm T|X has been set to English. It is possible to change this to French, German or Spanish, but the change should be made before the product is first used. Note that the Spectrum Analyzer software remains in English.

See the Read This First leaflet for instruction on changing the language.

17. Turning On and Turning Off

17.1. Palm T|X On/Off

General

The Palm T|X can be turned ON in either of two ways: by pressing the green button on the top edge, or by pressing any of the four keys below the display. Using the green button returns to the application in use when it was turned off. Using one of the four keys below the display will go to the application assigned to that key.

Note: When turning the unit back on, it may be necessary to press a key several times before it responds. This is because, in sleep mode, the keys are being polled very slowly as part of the power saving system.

The Palm T|X can be turned OFF by pressing the green button on the top edge. When operating on its battery and running standard Palm applications, it will turn off automatically after a short delay from the last action (settable between 30 seconds to 3 minutes). This automatic switch off is disabled whenever the mains adaptor/charger is connected (unless preferences are changed).

Within the PSAnalyzer Application

The PSA1301T is most easily switched on or off using the hard key marked Back. When using the PSAnalyzer application, pressing and holding this key for more than one second turns it off (sleep mode). Pressing it again turns it back on.

Note: It may be necessary to press the key more than once to turn on because of slow key polling in sleep mode.

The PSAnalyzer application suppresses automatic switch off of the Palm T|X and replaces it with its own battery saving system. Using the Auto Sleep function from the System menu, the unit can be set to turn off automatically at a user set delay between 5 minutes and 60 minutes from the last button press.

Any of the four main hard keys can be used to turn the unit on, though the Back (Home) key is preferable - because the other keys will also perform the function assigned to them. Alternatively the green button on the top edge can be used for on or off.

17.2. PSA1301 On/Off Control

The on/off state of the PSA1301 spectrum analyzer unit is controlled from the Palm T|X.

If the T|X is 'on' and the PSAnalyzer application is running, then the PSA1301 will be on. If the T|X is 'off', or if the T|X is on but an application other than PSAnalyzer is running, the PSA1301 will be off.

17.3. Operation Delay after Turning On

When the PSAnalyzer application is brought out of Sleep mode (by pressing a hard key or the green power key), the PSA1301 goes through a brief initialisation sequence. This can create a delay of up to two seconds during which the Run/Stop indicator turns red and shows Wait. It is also possible that the first sweep may be corrupted.

18. Battery and AC Power

The PSA1301T can operate using its internal rechargeable batteries, or from AC line using the adaptor provided by TTI.

18.1. Battery Operation

The Palm T|X and the PSA1301 incorporate their own rechargeable batteries. The AC adaptor/ charger provided by TTI recharges both batteries simultaneously. Charge control circuitry ensures that the batteries will not be over charged.



The PSAnalyzer application provides battery condition indicators for both batteries, the left hand one is for the PSA1301 (providing only a low battery warning), while the right hand one is for the Palm T|X and incorporates a multi-stage 'fuel gauge' type battery indication.

In normal operation within the PSA1301T, the Palm T|X battery will discharge more quickly than the PSA1301 battery. The PSA1301 battery also has a shorter recharge time.

However, should the PSA1301 battery become fully discharged, communications between it and the Palm T|X will stop and the red "WAIT" symbol will become permanently on. In these circumstances the left hand battery indicator will disappear completely.

Battery life depends upon screen brightness, but should be between three and five hours of continuous operation from a charge. Recharge time is typically less than four hours.

To conserve the battery the PSAnalyzer application can be put into sleep mode when not in use by pressing and holding the Home/Back key. Also auto-sleep mode can be selected whereby the unit turns off automatically after a defined period from the last key press. All data is retained when off.

Checking the Palm T|X battery condition


The precise condition of the T|X battery can be checked from within PSAnalyzer by accessing the Task Bar.

To display the task bar, press the Help key.

The task bar is displayed below the help screen text.



To check the battery condition select the "System Info" icon from the Task Bar. Press the Home key to exit.

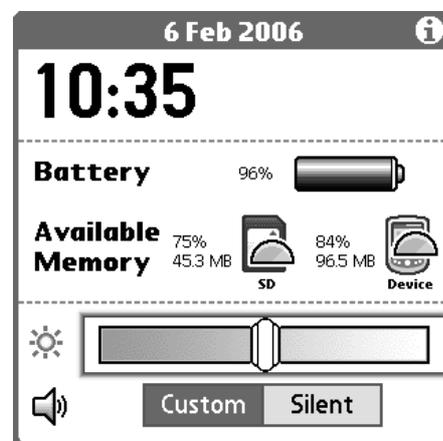

18.2. AC Power Operation

The AC adaptor/charger provided by TTI can be used as the permanent power source for the PSA1301T. If the batteries require re-charging, this will be done automatically and charging terminated at the appropriate point.



Use only the AC power adaptor provided by TTI. Use of any other power source could cause damage and will void the warranty.

When connected to the external power source, the right hand battery indicator will show a lightning" symbol.



Auto-sleep switch-off is disabled when external power is connected.

The LED next to the DC power input will illuminate while the PSA1301 batteries are charging.

18.3. Extended Periods Without Use

If the unit is left unused for extended periods, the batteries of both the Palm T|X and PSA1301 will gradually discharge. If the internal battery of the Palm T|X discharges beyond a certain point, re-initialisation will be necessary, see section [15](#).

The discharge time for either battery is typically several weeks, but could be considerably less if the batteries were already partly discharged when it was turned off.

If an extended period without use is envisaged, it is advisable to leave the unit connected to its charger in order to maintain the battery charge level.

19. Using the PSAnalyzer Application

19.1. Initial Conditions

The signal to be measured should be connected using the SMA connector at the top of the unit see section [11.1](#).



Signals that could exceed +20dBm (2.2V rms) or 15V DC, should be connected via a suitable attenuator. Signals exceeding this level could cause damage.

- ! Bluetooth or WiFi on the Palm T|X should be set to Off. (The very close proximity to the spectrum analyzer of a UHF source could cause spurious signals to be displayed).

To check that both wireless sources are off, press Help and observe the task bar at the bottom of the screen. The Bluetooth symbol should both be grey (rather than white). The WiFi symbol should show the word Wi-Fi rather than signal level bars. If not, select them from the task bar and turn the function off.



- ! The USB lead should be unplugged at the spectrum analyzer end. (The USB cable could induce interference into the spectrum analyzer that could cause spurious signals to be displayed).

19.2. Selecting and Leaving the Application

To launch the PSAnalyzer application, enter the Applications screen (by pressing the Home key once or twice). Press the PSAnalyzer icon (using the touch screen), or select it by pressing the centre button of the 5-way navigator twice.



To leave the application in order to use other Palm applications, select Exit from the main (home) menu and then use Exit Application.

19.3. Touch Screen or Hard Key operation

Handheld computer applications are normally operated using the touch screen. Most commonly they require the use of the supplied stylus because they involve selecting tiny icons or characters, or positioning a cursor precisely within a document.

The PSAnalyzer application has been written to give the user a choice - touch screen operation using a stylus or a finger tip, or hard key operation without ever touching the screen. These options are always present allowing the user to change operation method whenever they choose.

Touch Screen Operation


PSAnalyzer creates soft keys on the screen which are large enough to be operated using a finger tip as well as a stylus. Most functions are controlled directly using these soft keys, but some functions (such as scrolling digits or moving markers) are performed using the hard keys of the 5-way navigator. The basic functions of Run, Stop, Help and Back (Home) are also assigned to hard keys.

Hard Key Only Operation

Some users may prefer never to use the touch screen. PSAnalyzer allows all functions ** to be operated using only the hard keys. Each function is selected from the on-screen menus by scrolling through the keys using the 5-way navigator and pressing the central button. The currently selected key is shown by either a darker colour, or by a coloured outline. All menus including numeric entry screens can be operated in this way.

** It is not possible to enter user-defined file names using hard keys, default file names must be accepted instead. User-defined file names require the use of the Palm on-screen keyboard which can only practicably be operated using a stylus.

19.4. The PSAnalyzer Screen

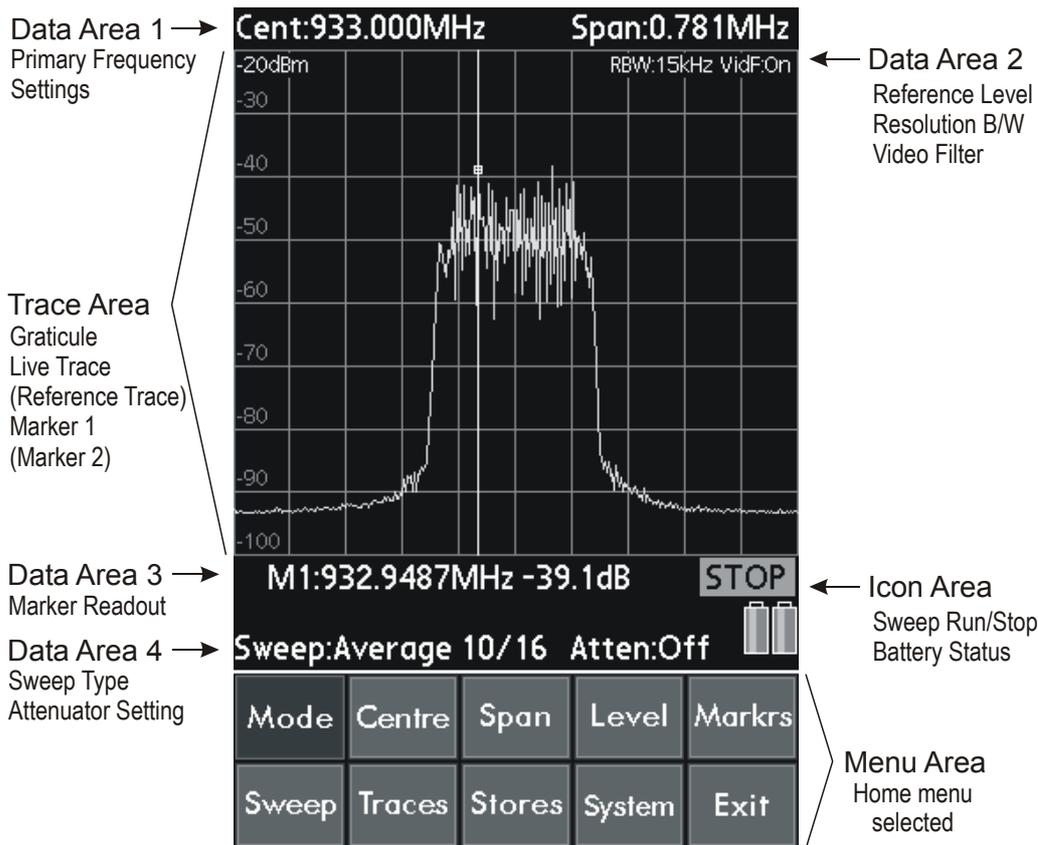

19.5. Operation and Navigation

The Palm T|X has nine hard keys (four dedicated keys plus the five way navigator). The PSAnalyzer application creates soft keys within a menu structure. Soft keys can be pressed directly (using a finger tip or stylus) or they can be operated using the five way navigator (left/right/up/down to select, centre to “press” the key). This latter mode avoids ever having to touch the screen.

The four dedicated keys are used to start or stop the sweep (Run and Stop), select context sensitive Help, and exit a sub menu and return to the home menu (Back / Home).

19.6. Turning Off / Power Saving

When operating from batteries the unit should be turned off when not in use. Press and hold the Back (Home) key. The display will go off, the status of the instrument is not lost and all data is retained apart from any running sweep. To turn back on, press the Back (Home) key again *. Alternatively use the recessed green on/off key on the top edge of the Palm T1X.

Note: an Auto Sleep function that automatically turns the unit off after a delay is available - see System menu, section [20.15](#). Auto Sleep is disabled whenever external power is connected.

* **Note:** When turning the unit back on, it may be necessary to press the key several times before it responds. This is because, in sleep mode, the keys are being polled very slowly as part of the power saving system.

20. The PSAnalyzer Menu System


20.1. Home Menu

Mode	Centre	Span	Level	Markrs
Sweep	Traces	Stores	System	Exit

All functions are operated from one of ten sub-menus selected from the Home Menu. To exit a sub menu and return to the home menu, press the Back (Home) hard key.

Alternatively pressing the area on the left hand side directly above the key row of a sub menu duplicates the action of the Back (Home) key. When using a stylus this may be more convenient than using the hard key.

This hidden key exists in all menus apart from the Home menu.

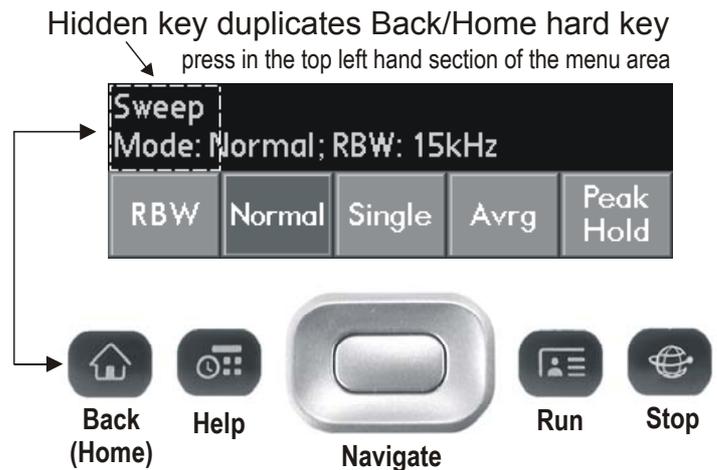

20.2. Menu Summary

Mode: set the control mode to Centre plus Span, or Start plus Stop, or centre plus demodulation (Zero Span). Also provides a function called Preset which sets defined conditions from a single key press. Note that the labels of the next two keys depend upon the mode setting.

Centre: set the centre frequency of the sweep (not available when mode = Start/Stop). A further sub menu of Set Step Value can be selected from the Centre menu.

Span: set the span of the sweep (not available when mode = Start/Stop).

Start or Stop: set the start or stop frequency of the sweep (not available when mode = Centre/Span or Zero Span).

AM/FM: set the type of audio demodulation for Zero Span mode (not available when mode = Centre/Span or Start/Stop).

Level: set reference level (by turning attenuator on or off); select vertical zoom and pan.

Markrs: set marker(s) on/off and position markers manually or automatically.

Sweep: select sweep mode (Single, Normal (continuous), Peak Hold or Average), set RBW (resolution bandwidth).

Traces: select Live and Reference traces, copy Live to Reference, set Video Filter, choose Hi or Lo resolution.

Stores: store or recall a trace or a set-up, copy a whole screen to an image file.

System: set auto sleep mode, set sweep averaging, turn graticule on or off.

Exit: exit from the PSAnalyzer application or suspend the application (sleep mode); view information about the application.

20.3. Mode Menu



This menu allows the selection of three different modes: Centre/Span, Start/Stop and Zero Span. The current mode is shown within the menu area. To change mode press the appropriate key after which the unit returns automatically to the home menu.

(Note that the two keys of the home menu to the right of the Mode key change depending upon the mode selected).

Centre/Span and Start/Stop are essentially the same mode, but with different options of control over the sweep parameters. When the mode is changed the sweep will remain the same and the values of start and stop or centre and span will be calculated from the existing sweep parameters.

Zero Span mode disables the sweep and shows a horizontal line representing the level at the centre frequency. AM or FM audio modulation is selectable with the audio available from a 3.5mm jack socket. Demodulation mode and audio level are selected from the AM/FM menu.

Preset is used to set a defined set of conditions from a single key press. It is particularly useful when the frequency location and level of the signal to be measure is unknown. Pressing Preset sets the following conditions:

Mode = Start/Stop, Start = 0.15MHz, Stop = 1300MHz, Sweep = Normal (and running), RBW = 280 kHz, Live Trace = On, Ref Trace = Off, Video Filter = On, Level zoom = Off (10dB/div), Attenuator = On, Graticule = On, Markers = M1 at 25%, M2 at 75%.

20.4. Centre Menu



This menu allows the centre frequency of the sweep to be set. Values are always in MHz with a maximum resolution of 0.001 (1kHz). The range is 0.310 to 1299.840 MHz. The current centre frequency is displayed within the menu area.

There are four ways to set the centre frequency:

Step Up/Step Down: allows the centre frequency to be increased or decreased in fixed steps as set by the Set Step Value sub menu which is accessed from this menu.

Set C = M1: sets the centre frequency equal to the frequency at the position of Marker One, and moves the marker to the centre of the graticule.

Set by Keybd: this opens a 0 to 9 numeric entry keypad. Keys can be pressed directly (with finger tip or stylus) or operated with the five way navigator. Press OK to activate the new frequency and return to the Home menu, or Cancel to escape.

Note: If Set by Keybd was the last function used within a menu, then it will be automatically selected the next time that the menu is entered.

Set by Tab/Jog: selects a numeric entry mode whereby the digits of the current centre frequency can be selected and incremented/decremented using the five way navigator. The changed frequency is activated automatically after a short delay. To exit this entry mode press the Back (Home) key.

(Note that when using a stylus, the digit to be “jogged” can be directly selected by pressing it).

Note: If Set by Tab/Jog was the last function used within a menu, then it will be automatically selected the next time that the menu is entered.

To exit this menu and return to the home menu press the Back (Home) key.

20.5. Step Value Sub Menu



This is a sub-menu of the centre menu. It sets the step value that will be used in the Step Up/Step Down function of the centre frequency menu. Values are always in MHz with a maximum resolution of 0.001 (1kHz). The range is 0.001 MHz to 100.000 MHz. The current step value is displayed within the menu area.

There are four ways to set the step value:

Set Step = M delta: sets the step value equal to the absolute value of frequency difference between the two marker positions.

Set Step = Span/10: sets the step value equal to one tenth of the current frequency span (i.e. one graticule division).


Set by Keyboard:

Set by Tab/Jog:

These two keys operate in the same manner as described for the Centre menu, see section [20.4](#).

To exit this sub menu and return to the centre frequency menu press the Back (Home) key.

20.6. Span Menu

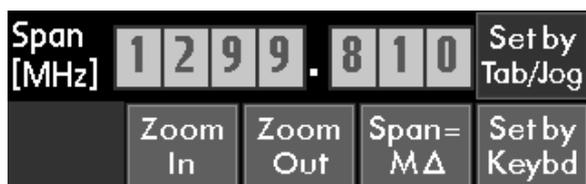

This menu allows the span of the sweep to be set. Values are always in MHz with a maximum resolution of 0.001 (1kHz). The range is 0.320 to 1299.850 MHz. The current span is displayed within the menu area.

There are four ways to set the span:

Zoom In/Zoom Out: decreases or increases the span in binary steps.

Span = M delta: sets the span equal to the absolute value of frequency difference between the two marker positions..

Set by Keyboard:

Set by Tab/Jog:

These two keys operate in the same manner as described for the Centre menu, see section [20.4](#).

To exit this menu and return to the home menu press the Back (Home) key.

20.7. Start Frequency Menu



This menu allows the start frequency of the sweep to be set. Values are always in MHz with a maximum resolution of 0.001 (1kHz). The range is 0.150 to 1299.680 MHz. The current start frequency is displayed within the menu area.

There are four ways to set the start frequency:

Start = M1: sets the start frequency equal to the frequency at the position of Marker One.

Start = M1/Stop = M2: sets the start frequency equal to the frequency at the position of Marker One and the stop frequency equal to the frequency at the position of Marker Two (both markers must be active for this function to operate)

Set by Keyboard:

Set by Tab/Jog:

These two keys operate in the same manner as described for the Centre menu, see section [20.4](#).

To exit this menu and return to the home menu press the Back (Home) key.

20.8. Stop Frequency Menu



This menu allows the stop frequency of the sweep to be set. Values are always in MHz with a maximum resolution of 0.001 (1kHz). The range is 0.470 to 1300.000 MHz. The current stop frequency is displayed within the menu area.

There are three ways to set the stop frequency:

Stop = M1: sets the stop frequency equal to the frequency at the position of Marker One.

Start = M1/Stop = M2: sets the start frequency equal to the frequency at the position of Marker One and the stop frequency equal to the frequency at the position of Marker Two (both markers must be active for this function to operate)

Set by Keyboard:

Set by Tab/Jog:

These two keys operate in the same manner as described for the Centre menu, see section [20.4](#).

To exit this menu and return to the home menu press the Back (Home) key.

20.9. AM/FM Menu




This menu controls the settings for demodulated audio in Zero Span mode, which can be Off, AM, or FM. The demodulated audio is outputted from the 3.5mm stereo/mono jack socket.

To change the volume press the Audio Volume key and use the up and down keys of the five way navigator to change the volume level (range 1 to 16).

To exit this menu and return to the home menu press the Back (Home) key.

20.10. Level Menu

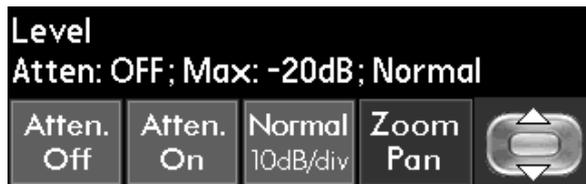

This menu allows the reference level (the level represented by the top of the graticule) to be changed by means of a switchable attenuator. It also allows the display to be vertically zoomed. The current status is shown within the menu area.

Atten. Off: turns the input attenuator Off and sets the reference level to -20dBm.

Atten. On: turns the input attenuator On and sets the reference level to 0dBm.

Normal: the normal level display is 10dB/div allowing the full 80dB display range to be shown. Use this key to cancel zoom mode.

Zoom/Pan: this key increases the vertical scale to 5dB/div. Use the up/down keys of the five way navigator to pan the 40dB window through the 80dB range.

To exit this menu and return to the home menu press the Back (Home) key.

20.11. Markers Menu



This is not truly a menu as it has no soft keys. Two markers are available shown by yellow and blue vertical lines. The frequency and amplitude at each marker point is displayed below the trace area, along with difference values. The five way navigator is used to control the markers as follows:

Turn Markers On - press the centre of the 5-way navigator to turn on each marker. (Note that only M1 or M1+M2 can be displayed - not M2 alone).

Select Marker to be Controlled - once both markers are displayed, subsequent presses of the centre key toggles the marker under control (shown in text and by an arrow in front of the selected readout).

Move Markers Left or Right - press the left and right navigator keys to scroll the selected marker. Auto speed-up is provided. Alternatively press the screen at the point that you want the selected marker to move to.



Find next Peak - press the up or down navigator keys to move the selected marker to the next higher or next lower amplitude peak.

Note: This function is peak tracking and will therefore follow the peak if the frequency is changing. To cancel peak tracking press the left or right navigator keys once.

Turn Markers Off - press and hold the navigator centre key to turn off each marker (M2 will turn off first).

To exit this function and return to the home menu press the Back (Home) key.

Note: Markers maintain a fixed position on the screen. Changing any sweep parameter (Start, Stop, Centre, Span) will change the frequency at marker position. The exception to this is the C = M1 function which also repositions the marker at the new centre frequency, see section [20.4](#).

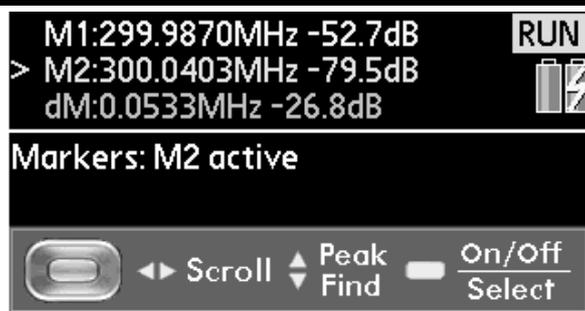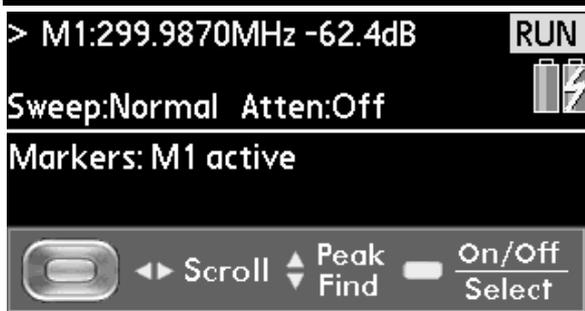

Note that, when both markers are selected, the display of sweep parameters and attenuator setting (data area 4) is removed and replaced by the marker difference values.

20.12. Sweep Menu



This menu allows the selection of four different sweep modes, and the setting of the resolution bandwidth (RBW). The current sweep mode and RBW are displayed within the menu area.

RBW: Toggles between the two resolution bandwidths of 280 kHz and 15 kHz.

Normal : sets a continuous sweep mode where a new sweep is commenced automatically after the previous sweep is completed. Press the Stop hard key to terminate the sweep and hold the trace on the screen. Press the Run hard key to restart sweeping.

Single: sets a single sweep mode whereby a sweep is initiated by pressing the Run hard key. When the sweep is completed the sweep stops and the trace is held on the screen.

Avrg: sets sweep averaging mode whereby the trace shows the average of a number of sweeps (selectable in binary steps 2 to 256). The most recent N sweeps are averaged, pressing Run restarts averaging from zero. Pressing Stop holds the trace. The averaging number is set in the System menu.

Peak Hold: in peak hold mode the trace shows the highest level detected at each frequency since sweeping was commenced. Pressing Run resets Peak Hold. Pressing Stop holds the trace.

To exit this menu and return to the home menu press the Back (Home) key.

20.13. Traces Menu



This menu allows the live trace and the reference trace to be turned on and off and the live trace to be copied to the reference trace. It also allows the screen resolution for the trace area to be changed, and the video filter function to be turned on or off. The current status is shown within the menu area.

Live Trace: toggles the live trace on and off - the live trace (green) is updated by the sweep function.

Ref. Trace: toggles the reference trace on or off - the reference trace (purple) can be either recalled from memory or copied from the live trace. If no reference trace has been created or recalled, the key will have no function.

Note: If the sweep parameters (start/stop or centre/span) are different from their values when the reference trace was captured, the trace is automatically shifted and scaled so as to correctly represent the stored trace for the new frequency span. The trace may therefore occupy only a part of the screen or may be off the screen altogether. An off-screen trace is indicated by a purple arrow at the appropriate edge of the graticule.


Live > Ref.: copies the live trace, as currently displayed on the screen, onto the reference trace.

Hi Res/Lo Res: toggles the screen resolution of the trace area. Hi Res uses 320 x 300 pixels, Lo Res uses 160 x 150 points where each point is 4 pixels; this provides thicker lines but less resolution.

Video Filter: toggles the video filter function on or off. When on, an analogue filter is applied to the trace which attenuates sudden transitions and noise.

To exit this menu and return to the home menu press the Back (Home) key.

20.14. Stores Menu

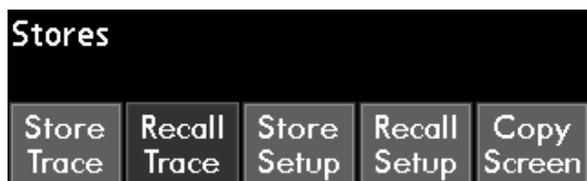

Traces can be stored to memory as files of amplitude and frequency (comma-separated-variable format). These files can be recalled to the reference trace. The complete set-up of the instrument can be saved to files for recall later. The whole screen (traces, graticule, annotation) can be stored to a bit-map image file for viewing or printing outside of the application.

Each key brings up a dialogue box which includes a scrollable window of existing files, a line for the currently selected file name, and three keys - OK, Cancel and Delete.

When a file is being stored, a default filename is allocated. This can be overwritten using the on-screen keyboard. Existing files can be overwritten by selecting them from the files window and pressing OK (a warning message is displayed).

Existing files can also be deleted by selecting them from the files window and pressing Delete (a warning message is displayed).

Note: The store, recall and copy functions are only available when the memory card is inserted.

Store Trace: press this key to store the live trace, as currently displayed on the screen, into a memory location. Opens a window showing existing stored traces and a default file name (e.g. trce001). Over-write file name, if preferred, using on-screen keyboard. Press OK to store.

Recall Trace: press this key to recall a stored trace to the reference trace. Opens a window showing existing stored traces which can be selected directly on-screen or via the 5-way navigator . Press OK to confirm recall.

Store Setup: press this key to store the complete set-up of the instrument into a memory location. Opens a window showing existing stored set-ups and a default file name (e.g. sett001). Over-write file name, if preferred, using on-screen keyboard. Press OK to store.

Recall Setup: press this key to recall a stored setup. Opens a window showing existing stored setups which can be selected directly on-screen or via the 5-way navigator . Press OK to confirm recall.

Copy Screen: copies the whole visible screen (from above the menu area) to a bit-map image file. Opens a window showing existing stored screens and a default file name (e.g. scrn001). Over-write file name, if preferred, using on-screen keyboard. Press OK to store.

To exit this menu and return to the home menu press the Back (Home) key.

20.15. System Menu



This menu is used to set the graticule display, set the averaging number for sweep averaging, and to set the delay time for auto sleep. The factory default set-up status can also be reloaded. The current status is shown within the menu area.

Avrg: press to set the number of sweeps that will be averaged when averaging mode is selected in the sweep menu. Use the up/down keys of the five way navigator to set the number (2 to 256 in binary steps).

Auto Sleep: press to set whether the unit goes into sleep mode (off) after a delay from the last key press. Use the up/down keys of the five way navigator to set either Off, or a time between 5 mins and 60 mins.

Auto-sleep is disabled when external power is connected.


Gratic. On/Off: press to cycle the graticule through three states: full on, horizontal lines only, off.

Reload Defaults: press to reload the instrument set-up status as shipped from the factory. (See section [24.1](#) - for list of factory defaults.

! **Calib.:** press to enter instrument calibration mode. Re-calibration can only be undertaken with specialised equipment and in conjunction with the Service Manual which is available from TTI.

To exit this menu and return to the home menu press the Back (Home) key.

20.16. Exit Menu

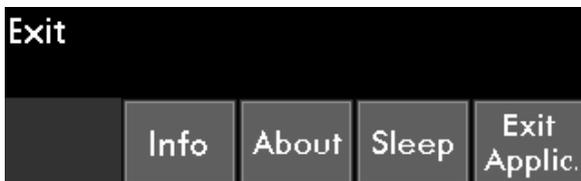

This menu allows you to exit from the PSAnalyzer application or suspend the application (sleep mode); and to view information about the application

Info.: Read a summary of the capabilities and specifications of the spectrum analyzer.

About: view information about this application (e.g. version number)

Sleep: turn off the application to save power - all current settings and data are retained. Press any of the four main hard keys, or the green button at the top of the unit to resume the application.

The unit can also be turned off (Sleep mode) by pressing and holding the Home hard key for > 1 second.

Note that the unit can be set to enter Sleep mode automatically after a fixed time - see System menu.

Exit Applic.: exit the application and go to the home menu of the Palm PDA. To re-launch the application find PSAnalyzer in the Palm T|X applications screen.

To exit this menu and return to the home menu press the Back (Home) key.

21. PSAnalyzer Operating Techniques

The following section contains some tips and hints regarding the operation of the PSA1301T. Each individual menu function is detailed within section 20 "The PSAnalyzer Menu System". Information is also provided in the context sensitive Help on the instrument.

21.1. Menu Navigation

The Hidden Key: PSAnalyzer is controlled via the ten operating menus, see section 20. Moving between menus requires a return to the Home menu by pressing the Back (Home) hard key. When using the touch screen for control (rather than the 5-way navigator), it is also possible to use the "hidden" key at the top LH side of each menu. This duplicates the action of the Back (Home) hard key.



The Menu Highlight Position: When using the 5-way navigator for control, pressing the select button operates the currently highlighted key. On leaving a menu, this position is remembered and is recalled when the menu is next entered. Thus, if Start = M1 was the last function used within the Start menu, it can be operated again by highlighting Start in the Home menu and pressing the selector button twice.

21.2. Frequency Setting

21.2.1. Centre/Span and Start/Stop modes

PSAnalyzer has three "modes" of operation selected from the Mode menu: Centre/Span, Start/Stop, and Zero Span.

Centre/Span and Start/Stop are not actually different sweep. Rather, they are different modes for setting and displaying the sweep parameters. The user can change between these two modes at any time without altering the sweep (apart from causing it to restart). The only effect will be to change the information directly above the graticule area, and the two menu keys to the right of the Mode key.

21.2.2. Centre Menu Shortcuts

Set Centre to Marker: To re-centre the sweep to a new position within the currently visible sweep, move the marker (M1) to the desired position and press Set C = M1.

Step Up / Step Down: The centre frequency can be moved in fixed steps (settable between 1kHz and 100MHz) by these two keys. The Set Step Val. key accesses the menu for setting the step size.

Step Value Shortcuts: The Step Value sub menu provides two shortcut keys. Step = M Δ sets the step size to the difference between the two marker positions M1 and M2. Step = Span/10 sets the step size equal to one tenth of the current span i.e. one graticule division.

21.2.3. Span Menu Shortcuts

Zoom In / Zoom Out: The span can be increased or decreased in binary steps by these keys.

Set Span equal to Marker Difference: The Spn = M Δ key sets the span equal to the difference between the two marker positions M1 and M2.

21.2.4. Start and Stop Menu Shortcuts

Set Start and/or Stop to Markers: The Start = M1 key moves the start frequency to the current position of marker M1. An equivalent functions is available from the Stop menu. The Strt=M1/Stp=M2 key sets the start and stop frequencies to the current marker positions.

21.2.5. Setting by Direct Numeric Entry

Each frequency related menu has a Set by Keybd key. This creates a 0 to 9 numeric entry keypad of large keys which can be pressed directly with the finger tip. (Alternatively they can be operated with the five way navigator). The entered value appears at the top.

The space below the keys contains the standard Palm input area. If required, this can be used to edit the number after it is entered and before it is confirmed using standard Palm cursor-based editing. See section [21.10](#) for details of how to change the input area type.

Press OK to activate the new frequency and return to the menu, or Cancel to abort and return to the menu. Note that the Back (Home) hard key does not operate within this screen.

If Set by Keybd was the last function used within a menu, then it will be automatically selected the next time that the menu is entered. This reduces the number of key presses required when entering new frequencies repetitively.

21.2.6. Setting by Tab and Jog

Setting by Tab/Jog provides an alternative to settings frequencies by the Keyboard. It is particularly relevant to users who wish to operate the PSA1301T without using the touch screen, but it is potentially relevant to all users.

Within any frequency menu, the current set frequency is displayed above the keys in a set of boxes. The Set by Tab/Jog function allows the frequency to be changed using the 5-way navigator (left/right to select digit, up/down to change digit). It is also possible to select the digit to be changed simply by using the stylus or finger tip to press it.

This also provides a quick and convenient way of stepping frequencies (although the step size is limited to decade values).

New frequencies do not have to be confirmed. A delay of about half a second is included between a digit being altered and the sweep parameters being changed to match. This allows digits to be scrolled without the sweep continually restarting.

If Set by Tab/Jog was the last function used within a menu, then it will be automatically selected the next time that the menu is entered. This reduces the number of key presses required when entering new frequencies repetitively.

21.3. Performing Sweeps

Frequency sweeps are started and stopped using the hard keys Run and Stop. The Sweep menu permits four different sweep types to be selected, and allows the resolution bandwidth to be changed, see section [20.12](#).

The Stop key halts the sweep at any time and holds the trace. The Run key initiates a new sweep and also resets Averaging and Peak Hold sweep modes. (Note that the averaging value is selected from the System menu rather than the Sweep menu).

When the sweep is in Stop, any change to the sweep frequency settings or to the attenuator setting will initiate a new single sweep. This is done to ensure that the live trace remains correct relative to the graticule markings.

Sweep Rate

There is no user control of the sweep rate. The speed of sweeping is determined by the frequency span and the resolution bandwidth; the analyzer sweeps at the fastest rate possible for the Span and RBW selected, subject to a maximum rate of approximately 5Hz.

The approximate sweep time can be calculated from the following formulae (span in MHz):

For RBW = 280kHz, sweep time = 200ms + (span x 8ms)

For RBW = 15kHz, sweep time = 200ms + (span x 80ms)

Thus, for example, a sweep of 10MHz span at 15kHz RBW will take about 1 second; whilst a sweep of 1GHz span at 280kHz RBW will take around 8 seconds.

Video Filter

The video filter has only two settings, on or off. The setting has no effect on the sweep rate.

By default the video filter is turned On. At 280kHz RBW this reduces the effects of system noise within the PSA1301 and improves the identification of low level signals just above the noise floor. The filter attenuates noise signals above about 10kHz. It has a negligible effect on peak amplitude measurements for signals at -60dB below the reference level or higher.

Where users wish to evaluate the noise performance of the system under test, they may wish to turn the video filter Off.

At 15kHz RBW the effect of the video filter is small.

21.4. Level Measurements

The normal display has a range of 80 dBs down from the top of the graticule (the reference level). The reference level is set from the Level menu, see section [20.10](#). With the attenuator off, the reference level is -20dBm, with the attenuator on it is 0dBm.

Note that any signal levels above the reference level can cause non-linearity in the detectors which could affect the amplitude accuracy of other signals which are below the reference level.

! The absolute maximum signal level that can be applied without damage is specified as +20dBm.

The display can be vertically expanded using the Zoom/Pan function. Zoom has a single level of x2, and the 40dB window can be panned over the full range using the 5-way navigator. Note that this function is for viewing purposes only and provides no improvement in accuracy or resolution, the latter being fixed at 0.1dBm.

21.5. The PRESET Key

The Preset key is found within the Mode menu, see section [20.3](#). It has a yellow outline to signify that it changes several things simultaneously.

Preset is used to set a defined set of conditions from a single key press. It is particularly useful when the frequency and amplitude of the signal is unknown, or when the existing status of the unit is unknown as might be the case when the PSA1301T is being shared between several users, or.

Pressing Preset sets the following conditions: Mode = Start/Stop, Start = 0.15MHz, Stop = 1300MHz, Sweep = Normal (and running), RBW = 280 kHz, Live Trace = On, Ref Trace = Off, Video Filter = On, Level zoom = Off (10dB/div), Attenuator = On, Graticule = On, Markers = M1 at 25%, M2 at 75%.

21.6. Using Markers

Markers provide a numeric readout of amplitude and frequency. Activation and control of markers using the Markers menu is described in section [20.11](#).

Markers are vertical lines with a box that highlights the intersection point of the marker with the trace. The readout shows the frequency and level at the intersection point. When both markers are displayed, the frequency and amplitude difference is also displayed. Markers provide an amplitude readout for the live trace only.

Markers also provide a quick and accurate method of resetting centre, span, start or stop frequencies to examine an area of interest. See section [21.2](#).

Although the frequency readout has a resolution of 0.1kHz, the uncertainty of the frequency at any sweep point is related to the span, being approximately 0.3% of the span width (span/320).

Note that markers retain their position relative to the graticule. When the sweep range is changed, the marker frequencies change with them.

Peak Find and Track: The Peak Find function (5-way navigator up/down) will automatically move the selected marker to the position of the highest amplitude peak. Thereafter pressing navigator down will move the marker to the next amplitude peak (regardless of its position on the screen), and so on downwards in amplitude. Pressing navigator up will move it through peaks of increasing amplitude.

The function will automatically track the signal. For each new sweep, the marker moves to follow its current peak position. If it is currently marking the third highest amplitude level, it will move to the position of the new third highest amplitude level when the signal changes. Only the currently selected marker will peak track.

Peak find/track is cancelled when the marker is moved manually, the selected marker is changed, or when any sweep parameter is changed.

Marker Movement Shortcut: When the Markers menu is selected, the active marker can be moved by touching the screen at the desired position.

21.7. Reference Trace

A reference trace (in purple) is available in addition to the live trace. See Traces menu, section [20.13](#). The reference trace can be copied directly from the live trace, or recalled from a memory store.

Both the reference trace and the live trace can be toggled on or off from within the traces menu.

Note: If the sweep parameters (start/stop or centre/span) are different from their values when the reference trace was captured, the trace is automatically shifted and scaled so as to correctly represent the stored trace for the new frequency span. The trace may therefore occupy only a part of the screen or may be off the screen altogether. An off-screen reference trace is indicated by a purple arrow at the appropriate edge of the graticule.

The reference trace is also shifted and scaled to match changes in the attenuator setting or the vertical zoom and pan.

21.8. Store, Recall and Copy

PSAnalyzer provides the facility to store traces and complete instrument set-ups to a memory card and recall them as required. See Stores menu, section [20.14](#).

Each key within the Stores menu brings up a dialogue box which includes a scrollable window of existing files, a line for the currently selected file name, and three keys - OK, Cancel and Delete.


When a file is being stored, a default filename is allocated. This can be overwritten using the on-screen keyboard. The maximum length of the file name is, in practical terms, limited to the length of file name entry line. However longer name will be accepted although the last characters will not be visible while they are being entered.

Existing files can be overwritten by selecting them from the files window and pressing OK (a warning message is displayed).

Existing files can also be deleted by selecting them from the files window and pressing Delete (a warning message is displayed).

The Copy Screen key copies the whole screen to the memory card as a bitmap image.

There is no Recall function for screen images. Screens are viewed outside of the PSAnalyzer application using the Media application of the Palm T|X, see section [23.1](#).

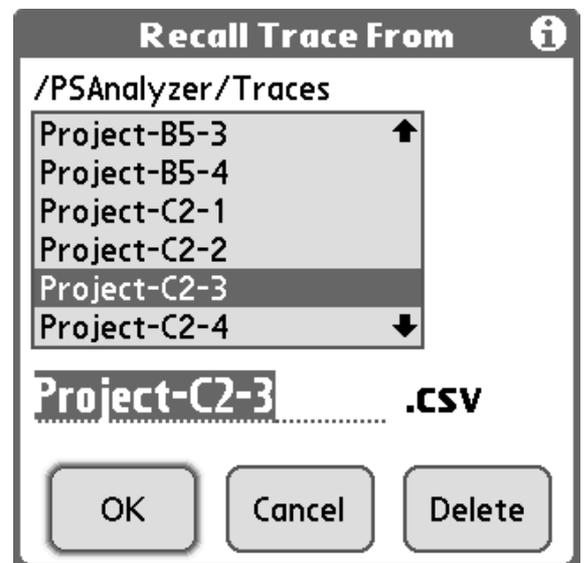

21.9. Screen Resolution and Trace Thickness

The high resolution of the Palm TjX screen (pixel spacing = 0.165mm) provides an excellent level of trace detail. However, because it is drawn one pixel wide, the trace is thin and may be difficult to view from a distance away.

If a thicker trace is required, the screen resolution can be changed from within the Traces menu, see section [20.13](#). In Lo Res. mode, the graticule area is modified to have only 160 x 150 points, where each point is made up of four pixels.


This lower resolution mode provides a thicker trace that halves the number of sweep points displayed while retaining peak detection. Pairs of points are combined into single points using the higher of the two amplitudes. Note that the maximum frequency resolution of the marker is halved. Greater measurement accuracy will be achieved using Hi Res. Mode.

21.10. Changing the Palm Input Area type

The Set by Keyboard function for frequency setting, and all Store/Recall functions brings up the standard Palm input area at the bottom of the screen.

This input area can be alpha, numeric or graffiti.

To change the type, use the stylus to press one of the small graphics below it:

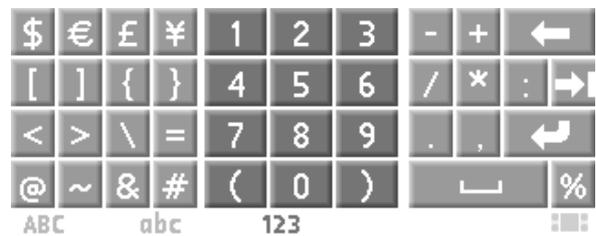

ABC = upper case letters, abc = lower case letters, 123 = numerics, the right-hand graphic = graffiti area.

21.11. Adjusting the Display Brightness

The display brightness can be adjusted from within PSAnalyzer by accessing the Task Bar. To display the task bar, press the Help key. The task bar is displayed below the help screen text.



To change the brightness select the “System Info” icon from the Task Bar (the icon which shows the time).

11:14

Set the brightness and then press the Home key to exit.

22. Help Screens

PSAnalyzer provides sixteen context sensitive Help screens. Each menu has its own associated help screen which may contain several pages of scrollable text.

Some general information about the specification and capabilities of the product is also available from the Info key under the Exit menu.

Help screens also provide access to the standard Palm Taskbar which allows the screen brightness to be changed and Palm system information to be checked (time, date, battery status, memory status, Wireless status and alerts). See sections [21.11](#) and [28.8.4](#).

Note: Help screens should be closed by pressing Done as soon as they have been read. When a Help screen is open, the PSAnalyzer application will turn off after the standard delay set within the Palm preferences (adjustable 30 secs to 3 mins).

23. Functions outside of PSAnalyzer

23.1. Viewing a Stored Screen Image

Screen images are stored from within the PSAnalyzer application, see section [20.14](#). However, to view or print a stored screen image, it is necessary to exit the PSAnalyzer application and use the native applications of the Palm TIX.

The following assumes that screens have been saved to the default position on the plug-in memory card (the folder DCIM \ PSAnalyzer).

Open the Media application from the Application screen, or use the Photos and Videos shortcut from the Favourites screen.

Ensure that the Card icon is selected (top right hand side) and set the drop down menu to either PSAnalyzer or All Albums. Thumbnails of available images will appear - this can be set (at the bottom left of the screen) to be thumbnails only or thumbnails plus file details.

Select the image to be viewed from the file list by pressing its thumbnail or its name (e.g. scrn001). After a few seconds the image will appear. Pressing anywhere on the screen will return to the thumbnails view. Press the home key to exit the Media application.

23.1.1. Adding Annotation to Screens

The Media application menu option "Draw on Picture" allows images to be annotated (using sketching and/or text) and then saved as a new image.

See the Palm TIX documentation for full information on the Media application.

23.2. Printing a Stored Screen Image (using a printer connected to a PC)

Screen image files are stored on the memory card in the DCIM \ PSAnalyzer folder and have the extension .bmp. See section [24.3](#) for more details.

To transfer a screen image to a PC for printing it is necessary to use the USB linked card reader supplied with the PSA1301T.

When transferred to a personal computer, screen image files can be opened in any image editing program, and by the Picture and Fax Viewer application of Windows XP from which printing can be initiated.

23.3. Transferring PSAnalyzer Files to a Personal Computer

PSAnalyzer uses a plug-in memory card to store screen images, traces and set-ups. There are three types of file; trace files, set-up files, and screen image files. All of these might be transferred onto a PC for backup purposes. In addition, screen image files may need to be transferred for printing, and trace files may be required for import into other programs such as Excel.

Trace files are stored on the card in the folder PSAnalyzer\Traces. Set-up files are stored on the card in the folder PSAnalyzer\Setups. Screen image files are stored on the card in the folder DCIM\PSAnalyzer. See section [24.3](#) for details of the file types and structures.

To transfer any file to a PC it is necessary to use the USB linked card reader supplied with the PSA1301T. Alternatively, any type of card reader that the user may already have can be used provided that it supports SD/MMC type cards.

! **Important** - Do NOT try to make a direct USB connection from the PSA1301T to a PC which has not had the Palm software loaded onto it in advance.

23.3.1. Using the Memory Card Reader

TTi provides a USB linked memory card reader to allow PSAnalyzer user files to be transferred to and from a personal computer.

The type of card reader supplied may vary from time to time. It may be a single card type (SD and MMC cards only) or a multi-card type. A USB extension lead may also be provided for card readers which do not have their own flexible connection lead.

Installation

No driver files should be required for installation under Windows XP, Windows 2000, Windows ME, or Mac OS9 or OS10. Installation under Windows 98 SE should also be possible, but it may be necessary to download drivers from the manufacturer's website.

Plugging the card reader into an unused USB port (USB 2 or USB 1) should cause the operating system to recognise the device and to load suitable drivers. This may take some time as more than one driver has to be installed. When installation is complete, the operating system may request a reboot.

The card reader is seen as a removable disk drive, and the operating system should automatically allocate it an unused drive letter. The device should be visible under Windows in My Computer.

In the event of difficulties see section [26.4](#).

Transferring Files

Once the installation procedure has been carried out, it will be possible to plug and unplug the card reader as required with the operating system automatically recognising it and allocating it a drive letter.

With the card inserted, open the "disk drive" under its allocated drive either from My Computer or from Explorer. The directory structure of the card will be visible. Trace files are stored in the folder PSAnalyzer\Traces. Set-up files are stored in the folder PSAnalyzer\Setups. Screen image files are stored in the folder DCIMPSAnalyzer. Files can be transferred between the card and the PC by using the normal drag and drop techniques.

23.4. Sending PSAnalyzer Files via Bluetooth or WiFi

The Palm TjX incorporates both Bluetooth and WiFi, allowing wireless connections to be made to a mobile phone, a personal computer, or a WiFi network.

Note: Setting up of WiFi and Bluetooth connections, and setting up Email are covered within the Palm documentation. TTI and their agents/distributors do NOT provide any support advice on these subjects.

23.4.1. Email Attachments

Any files stored on the memory card (as well as any data with the internal memory) can be selected as attachments to an email and sent to a remote or local computer.

23.4.2. Sending Images from the Media application

PSAnalyzer screen image files can be send directly from within the Media application using Bluetooth. Alternatively they can be beamed using IR.

23.4.3. Direct File Transfer using WiFile LT

Palm currently supplies a WiFi file sharing program called WiFile LT on the support CD. This may provide the capability to move files to and from shared folders on a computer within a network.

Note: Both Bluetooth and WiFi must be turned OFF when using the spectrum analyzer in active sweeping mode.

24. PSAnalyzer Files and Defaults

24.1. Factory Default Settings for PSAnalyzer

As initially supplied, the set-up of the spectrum analyzer is as follows:

Mode = Start/Stop. Start frequency = 0.15MHz, Stop frequency = 1300MHz
Attenuator = On (reference level = 0 dBm). Level zoom = Off (10dB/div)
Sweep = Normal (and running). RBW (resolution bandwidth) = 280 kHz
Live Trace = On. Ref. Trace = Off. Resolution (of trace area) = High Res. Video Filter = On
Markers = M1 set to On at centre frequency (M2 = Off)
Graticule = On, Averages = 16, Auto Sleep = 30 mins

These factory defaults can be reloaded at any time from within the System menu.

24.2. File Locations for PSAnalyzer data files

The PSAnalyzer application is stored within the internal program memory of the handheld computer. The initialisation file that stores the “last used” settings when the application is terminated is also stored within the internal memory. However, files created by the user (stored traces, set-ups and screens) are stored on a plug-in memory card.

Trace files are stored in the folder PSAnalyzer\Traces. Set-up files are stored in the folder PSAnalyzer\Setups. Screen image files are stored in the folder DCIM\PSAnalyzer.

24.3. File Structures for PSAnalyzer data files

Trace Files

Trace files have the extension .csv and are standard “comma separated variable” files suitable for import into Excel, MathCad or any other program that supports CSV import.

A file consists of 320 data pairs representing each frequency point in the trace. The first number is a frequency in MHz to four decimal places, e.g. 742.6830. The second number is the amplitude in dBm to one decimal place (amplitudes will be within the range 0.0 to -100.0).

Screen Files

Screen files have the extension .bmp and are bitmaps representing the whole of the screen above the menu area. Each file uses 120 kilobytes and is an image of 379 pixels high by 320 pixels wide in 8-bit indexed colour format.

When transferred to a personal computer, screen files can be opened in any image editing program, and by the Picture and Fax Viewer application of Windows XP.

Set-up Files

Set-up files have an encoded structure and have no function outside of the PSAnalyzer application. The only reason for transferring them onto a personal computer would be for back-up purposes. The file extension is .ini.

25. Maintenance, Calibration and Repair

25.1. Screen Protection

Handheld computers are sometimes used with Screen Protectors - a thin transparent film which covers the touch screen. When used in a clean environment using either a stylus or hard keys only, a Screen Protector is not necessary.

In dirty environments or when using a finger to press the screen, it may be advisable to use a Screen Protector to prevent grease or other contaminants from damaging the screen. A Screen Protector reduces the quality of the display somewhat, although this can be minimised by careful application.

Some people generate a considerable level of grease from their finger tips, and may find that the screen quickly becomes smeared when regularly touched. Other people may experience no difficulties from touching the screen without a Screen Protector in place.

Screen Protectors are available from a variety of sources.

25.2. Cleaning

If the unit requires cleaning, use a cloth that is only lightly dampened with water or a mild detergent. Take particular care in cleaning the touch screen area. Refer to the Palm documentation for further advice.

25.3. Maintaining Battery Condition

If left unused and disconnected for an extended period, the rechargeable batteries will discharge beyond the point where normal operation is possible. See Section [18.3](#).

If an extended period without use is envisaged, it is advisable to leave the unit connected to its charger in order to maintain the battery charge level.

25.4. Calibration

To ensure that the accuracy of the instrument remains within specification the calibration should be checked (and if necessary adjusted) annually. The calibration adjustment procedure is detailed in the service manual.

25.5. Service & Repair

Palm T|X handheld computer

Warranty and Service is the responsibility of Palm. In the event of a fault occurring, access your local Palm website for details of how to proceed. These websites are country specific, but can be accessed through the route web address of www.palm.com

PSA1301 Spectrum Analyzer Adaptor

TTi or their agents overseas will provide a repair service for any PSA1301 spectrum analyzer adaptor developing a fault.

Where owners wish to undertake their own maintenance work, this should only be done by skilled personnel in conjunction with the service manual which may be purchased directly from the TTI or their agents overseas.

26. Trouble Shooting

26.1. Correcting Unexpected Conditions in PSAnalyzer


If the PSAnalyzer application appears to be performing in an unexpected way, the following solutions should be tried.

1. Exit the PSAnalyzer application and restart it.
2. Recall a previously stored Set-up file from the Stores menu. (Store the current settings first if they are important).
3. Operate the Reset button on the PSA1301. This button is located on the right-hand side of the instrument, and should be operated using a thin non-metallic object such as a pencil tip.

This reset is non-destructive. It restarts the microprocessor in the PSA1301 but all set-up information is retained as this is reloaded from non-volatile memory after the reset.

Note that the button is too far recessed to be operated by the stylus tip. The original stylus supplied with the Palm T|X has a suitable thin point concealed within its cap. A replacement stylus may not have this.

4. Operate the Reload Defaults button on the System menu. This will restore the unit to its factory defaults as listed in section [24.1](#).
5. If none of the above corrects the problem, try resetting the Palm T|X as detailed below.

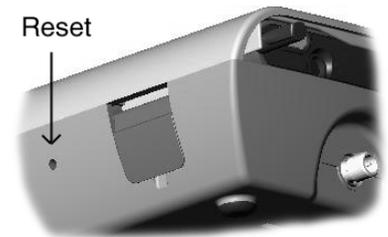

26.2. Resetting the Palm T|X

Handheld computers, such as the Palm T|X have a complex operating system which can occasionally “crash” or otherwise cease to operate normally. Should this happen, it will be necessary to perform a reset procedure. There are two types of reset, a soft reset and a hard reset.

Performing a Soft Reset


Remove the Palm T|X from the PSA1301T (see section [14](#)). Use the stylus (or a similar object without a sharp tip) to gently press the reset button on the rear.

The screen will go blank briefly and then the operating system will reload as indicated by moving black bars.

It may be necessary to re-enter the time, date and location. However, no other data will be lost.

Performing a Hard Reset (Caution !)

Only do a hard reset if a soft reset doesn't solve your problem, or if you want to clear all of your information from your handheld.

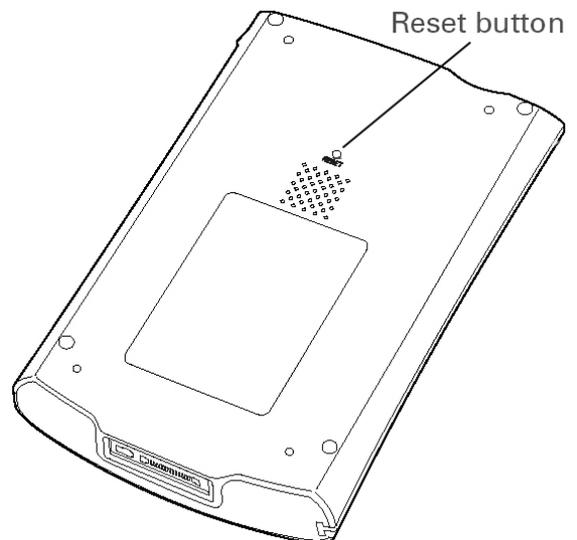

! A hard reset deletes all records and entries stored on your handheld, including the username that identifies the handheld. It will also erase the PSAnalyzer program and any other third party programs that are not incorporated within the permanent ROM memory of the device.

1. Press and hold the power button.
2. While holding the power button, use the tip of the stylus (or a similar object without a sharp tip) to gently press and release the reset button.

-
3. Wait for the Palm Powered™ logo to appear (not the first Palm logo that appears), and then release the power button.
 4. When you see the message that warns you about erasing all of the info on your handheld, do one of the following:
 - Press Up on the 5-way navigator to finish the reset and show the touchscreen,
 - or • Press any other button to do a soft reset.

26.3. Reinstalling or Updating the PSAnalyzer application

Creating a Duplicate Card

Reinstalling or updating the application may require the original memory card supplied with the PSA1301T by TTI. Should this have been lost or erased, it will be necessary to create a duplicate from the support CD supplied by TTI with the product.

Take a suitable SD or MMC card and insert it into a card reader connected to a PC.

Find or create a folder called Palm, then find or create a sub-folder called Launcher. Open the CD and open the folder Card\Palm\Launcher, then copy the file PSAInstaller.prc to the Launcher sub-folder on the card.

Find or create a folder called PSAnalyzer, then create a sub-folder called Software. Open the CD and open the folder Card\PSAnalyzer\Software, then copy the file PSAnalyzer.prc to the Software sub-folder on the card.

Reinstalling the Application

Should the PSAnalyzer application be erased by performing a Hard Reset or by any other means, it will be necessary to reinstall it. The memory card supplied with the PSA1301T includes a backup copy of the application and an Installer program.

Remove and re-insert the memory card supplied with the PSA1301T by TTI. The Applications screen will appear showing the utility program PSAInstaller. Select this program and follow the on-screen instructions.

When completed, return to the normal Applications screen by selecting the drop down menu at the top right and select "All" in place of "Card".

Updating the Application

From time to time TTI may issue updated versions of the PSAnalyzer application. These are likely to be made available via a web download. The version number of the currently installed PSAnalyzer can be checked from within the application by going to the Exit menu and selecting About.

Take the memory card supplied with the PSA1301T by TTI, and insert it into a card reader connected to the PC onto which the new version has been downloaded.

1. Locate the backup version of the program (PSAnalyzer.prc) in the folder PSAnalyzer\Software.
2. Create a new sub-directory called (say) Older, and move the older PSAnalyzer.prc into it.
3. Copy the new version of PSAnalyzer.prc to the folder PSAnalyzer\Software.

Re-insert the memory card. The Applications screen will appear showing the utility program PSAInstaller. Select this program and follow the on-screen instructions.

When completed, return to the normal Applications screen by selecting the drop down menu at the top right and select "All" in place of "Card".

26.4. Card Reader Installation Problems

Installation instructions are given in section [23.3.1](#) and may also be included with the device.

Early operating system such as Windows 95, Windows NT and the first version of Windows 98 do not support USB devices. Windows 98 SE does support USB but a driver may be required from the card reader manufacturer's website.

Once installed the card reader is seen as a removable disk drive, and the operating system should automatically allocate it an unused drive letter. The device should be visible under Windows within My Computer.

There are circumstances where installation appears to be perfectly normal, but the device does not become visible through My Computer. This is typically caused by a clash with a Network drive.

Should this occur, insert a card into the reader and open Control Panel > Administrative Tools > Computer Management > Disk Management (Windows XP/2000 only). Locate the card (disk) which can be identified by its description (removable), its filing system (FAT), and its size in MB. Right click it's disk icon and select "change drive letter and path". Change the drive letter to one that will not clash with any network drives or any removable drives that might be connected to the system at any time.

27. Support Information and Accessories

27.1. Support Information for the Palm T|X

TTi and its agents/distributors do NOT provide support for the Palm T|X other than for its use within the PSA1301T running the PSAnalyzer application.

A considerable amount of support information is provided in PDF form on the CDs included with the product.

The Software Installation CD supplied by Palm includes a Getting Started manual in English, French, German, Italian and Spanish, plus a simplified manual in several other languages.

The CD supplied with the PSA1301T by TTi includes the full Palm T|X manual (in English) within the directory \Palm.

Further support information is available from Palm websites. These websites are country specific, but can be accessed through the route web address of **www.palm.com**

A number of other non official websites and forums exist which may provide useful information. These can be found by using a search engine.

27.2. Standard Accessories supplied for the Palm T|X

A number of accessories for the Palm T|X are supplied by Palm within the shipping box. These include a USB HotSync lead, a universal voltage AC adaptor/charger, and a leather cover.

None of these items are useable with the PSA1301T, but can be used with the Palm T|X if it is removed.

The Palm T|X shipping box also contains the following:

License and Warranty Information

Printed "Read This First" Manual (multi language)

Software Installation and Support CD for Windows and Mac computers (multi language)

27.3. Optional Accessories

Optional Accessories for the PSA1301T

For a list of optional accessories for the PSA1301T, visit our website: **www.tti-test.com** or contact TTi directly.

Optional Accessories for the Palm T|X

A number of optional accessories are available for the Palm T|X, along with software applications. Palm websites are country specific, but can be accessed through the root web address:

www.palm.com

28. Appendix A.

Using other functions of the Palm T|X

NOTE: The following information is an overview of the functionality of the Palm T|X intended for PSA1301T users who are unfamiliar with such devices. It is not intended as a substitute for Palm's own documentation, and its accuracy is not guaranteed.

TTi (and its agents and distributors) do NOT provide technical support for any other functions of the Palm T|X outside of the PSAnalyzer software application. Technical support for all other functions must be obtained from Palm or from associated support websites. See section [27.1](#).

Users should refer to the full PDF instruction manual (TX_Handbook_en.pdf) which is included on the TTi PSA1301T support CD. A more recent version may be available from the Palm Website.

Multiple language version of a Getting Started manual are included on the Palm T|X Software Installation CD. These can be installed directly onto the Palm T|X itself, see section [28.7](#).

Useful basic information is also provided by the Quick Tour application on the Palm T|X and the "Discover Your Device" tutorial on the Palm installation CD.

28.1. Handhelds and PDAs - Overview

Devices such as the Palm T|X are described as hand-held computers, palm-top computers or PDAs (personal digital assistants). The origin of these devices lies in the personal organisers of the 1970s. Companies such as Palm (Palm Pilot) and Apple (Apple Newton) then developed much more powerful devices incorporating touch sensitive screens for stylus based operation, and operating systems that could run many types of software application..

Today's hand-held devices have powerful microprocessors, full colour high resolution screens, and application software capable of duplicating many of the functions of a full size personal computer.

28.2. Software provided by Palm on CD

None of the software and applications on the Palm T|X Software Installation CD are necessary for operation of the PSA1301T as a spectrum analyzer.

Palm provides extensive software for both Windows and Mac computers intended for sharing information between the Palm T|X and a PC. Some additional applications for the Palm T|X are also included on the CD.

28.3. Linking to a Personal Computer

It is NOT necessary ever to link the PSA1301T to a personal computer. However, some of the additional features of the Palm T|X do require linking to a personal computer in order to share information, load new software applications and transfer files. This will require the installation of the Palm Desktop software - see Appendix B, section [29](#).

Note that transferring PSAnalyzer files to a PC can NOT be done using Palm Desktop software. Files must be transferred using the memory card and a card reader. See section [23.3](#).

! **Important** - Do NOT try to make a USB connection to a PC which has not had the appropriate software loaded onto it. See next section.

28.3.1. USB connections to a PC

The following applies to both the PSA1301T and the Palm T|X by itself. The mini USB connection on the side of the PSA1301T is a direct through connection to the USB port of the Palm T|X.

As stated previously in this manual and in the Read This First leaflet, a direct USB connection should only be made to a PC if the user intends to use the Palm Desktop software on that computer. In that case, the Palm installation CD must be run on the computer prior to making the USB connection.

! Do NOT attempt to make a USB connection otherwise. The operating system is likely to identify a Palm device and to load a generic driver for it. This driver may be incompatible with the Palm T|X and may prevent correct operation of the Palm Desktop software thereafter.

USB transfer of PSAnalyzer user files can only be done using a memory card reader, see section [23.3](#). Direct USB file transfers using Palm Desktop software is only relevant to native Palm applications and full system backups.

28.4. Palm Desktop software

Palm Desktop is Palm's companion software application for linking the Palm T|X to a PC. It is a powerful piece of software which enables the user to maintain certain types of data simultaneously on the handheld computer and on the PC. It also provides facilities for document conversion, backup of data, and installation of new programs.

Palm Desktop software has no direct relevance to PSAnalyzer.

Users of the PSA1301T should read Appendix B, section [29](#) before deciding whether or how to install Palm Desktop.

28.5. Core Capabilities of the Palm T|X

The full functionality of the Palm T|X is defined by the installed Applications. These applications make use of the core capabilities of the product which are as follows.

Screen - High resolution 320x480 transfective TFT colour display, landscape or portrait mode, full area Touch Screen.

Processor - 312 MHz Intel Xscale processor.

Memory - 128MB of Flash memory (100MB available to user). Non-volatile, all data retained if battery is fully discharged.

Audio - Stereo out via 3.5mm 'phones socket, built-in loudspeaker.

Control - Touch screen operation from task bar, on-screen menus and drop-downs. Most functions can also be operated using only the 5-way navigator.

Text Input

Qwerty Keyboard - selectable on-screen keyboard for "typing" with the stylus.

Handwriting Recognition - built-in Graffiti-2 character recognition allows text entry by 'writing' on the screen.

Connectivity

USB for easy connection to personal computers.

Bluetooth for wireless connection to computers, mobile phones, and Bluetooth peripherals.

WiFi for wireless connection to computer networks (and wireless internet).

Infra Red for connection to other handheld/PDA devices, mobile phones, IR peripherals.

Expansion - slot for SD, SDIO and MMC cards.

28.6. Standard Applications

Standard applications are included within the permanent memory of the TIX. Note that the following list is illustrative only. Palm may vary the applications provided with the Palm TIX from time to time, and could omit one or more of the listed applications or add others.

Addit - commercial application intended to facilitate purchasing of additional software applications.

Calc - large key calculator suitable for fingertip operation. Standard, mathematical, financial, conversion, logic and statistical functions (press 5-way navigator > to change mode). Up to 14 digits of precision. Scrollable calculation history. Copy and paste results into applications.

Calendar - full appointments/tasks diary system with editable text, durations, reminders and alarms.

Card Info - provides summary details for any card plugged into the SD card slot.

Contacts - easily searchable contacts database with customisable storage for large amounts of information per person including thumbnail photographs.

Dialer - establish a bluetooth or IR connection to a mobile phone for dialling direct from the TIX. Copy and paste phone numbers from Contacts.

Documents - DataViz Documents-To-Go - provides compatibility with Microsoft Office documents in Word, Excel and Powerpoint.

Expense - provides a convenient method for recording and sorting expenses details and receipts.

Favourites - customisable list of applications, files, folders or web links that can be accessed directly.

HotSync - synchronises information between the TIX and a personal computer. The information to be synchronised can be set by the user. Particularly relevant to maintaining Calendar, Contacts and Expense data.

Media - application for viewing and organising photos and videos.

Memos - simple word processor application for creating text documents that do not require text formatting (otherwise use Documents).

Note Pad - enables drawings (hand writing, diagrams etc.) to be made on screen and saved.

Prefs - accesses the Preferences screen from which many functions of the TIX can be customised.

pTunes - MP3 music player application.

SMS - create SMS text messages to send via a mobile phone linked by Bluetooth or IR.

Solitaire - game application.

Tasks - create and maintain task lists linked to Calendar.

VersaMail - provides an email facility when Bluetooth or IR linked to a mobile phone or WiFi linked to a Network.

Web - opens a web browser (called Blazer) and accesses a WiFi or Bluetooth connection for internet access.

World Clock - provides a time and date display for three world locations chosen by the user.

28.7. Additional Applications

Palm provides some additional applications on the Palm T|X Software Installation CD,. These may include the following:

Getting Started Guide (Manual)- installs the Palm T|X basic operating manual onto the unit as an application.

WiFile LT - the “light” version of WiFile Pro. This is a file sharing program which provides the capability to move files to and from shared folders on any computer within a network using WiFi.

eReader - application for use with electronic books.

Acrobat Reader for Palm OS - allows standard Adobe Acrobat PDF files to be read. (Also installs a converter program onto the PC).

A number of other add-ons are provided on the CD. Some are PC based software to improve integration with Windows. Others are basically web links to enhancements or upgrades.

28.8. Some Palm Basics

28.8.1. Operating System, Memory and Filing System

The Palm T|X uses the Palm OS 5.4 operating system. This operating system uses a propriety database type filing system. Data stored in this filing system can not be viewed or accessed directly by a Windows based PC (or Mac). Transfer of data between the handheld computer and the PC requires Palm Desktop software to be installed.

The Palm operating system can also make use of memory with a conventional filing system. This memory is normally provided via a plug-in SD or MMC Flash memory card. Data on this card will use a conventional folder based filing system and has the potential to be viewed and accessed on a Windows or Mac PC.

Files created by most Palm applications and stored on a memory card will have the extension .prb (palm database). The content of these files can only be viewed on a PC by using Palm Desktop software. However, the Documents application can create files in Microsoft Office format (Word and Excel) that can be directly used on a PC.

The Palm T|X contains 128MB of Flash (non volatile) memory. 100MB of this memory is available to the user. By default this memory uses the Palm database filing system.

28.8.2. Modes of Operation

Palm applications are designed for operation using the touch screen and a stylus. A few applications (such as Calculator) can be operated using a finger tip in place of the stylus. Most applications also support some level of operation using the 5-way navigator thus enabling single handed operation.

Briefly tapping an icon selects it. Some icons have an alternative function that is selected by pressing and holding (though most do not). Editable text items have a cursor position which is selected by touching the screen. Multiple characters can be selected by pressing and dragging. Text can be entered using the on-screen keyboard (or by using hand writing recognition).

To use the 5-way navigator, press the centre button to create a highlight (unless a highlight is already present). Thereafter the navigator can be used to move the highlight and make selections. The operation of the navigator varies in different applications and may have some dedicated functionality.

Some menu options show a character short cut (e.g.  C for Copy). This refers to the use of the stylus within the handwriting input area and will only be of relevance to users who have learnt and regularly use handwriting recognition.

28.8.3. Hard Keys



By default, the four main hard keys of the T|X are set to launch the following applications (left to right): Home (Applications/Favourites), Calendar, Contacts, Web Browser. The function of the keys can be changed from within Preferences.

Home Key



The Home key - can be used in any standard Palm application to open either the Favourites screen or the Applications screen, depending upon the settings in Preferences. Further presses alternate between Applications and Favourites. Pressing and holding the home key brings up a menu of the most recently used applications.

The key also exits an application and terminates it (except for background applications such as pTunes).

28.8.4. Task Bar



The task bar is present in all standard Palm applications, occupying the bottom of the screen (or side of the screen in landscape mode). It is suppressed within the PSAnalyzer application in order to maximise screen area, however, it can be temporarily enabled by entering a Help screen.



Find - search for data by name. (The Find function will only find data that is directly related to a standard Palm application).



Menu - displays one or more drop-down menus giving options relevant to the current application.

Note that in most applications the Menu can also be accessed by pressing the identifier tab at the top left hand side of the application screen.



System Info - show time and date, battery condition, and available memory. Control screen brightness and sound on/off.



Alerts - if any alerts have occurred (e.g. a diary appointment) this will flash. Press to view.



Bluetooth - turn Bluetooth on or off, change Bluetooth preferences and set-up.



WiFi - turn WiFi on or off, change WiFi preferences and set-up.



Full-screen Writing - normally Graffiti handwriting recognition is limited to an area at the bottom of the screen. It can alternatively be enabled for the full screen area.



Screen Rotation - change the screen orientation from portrait to landscape or vice versa.



Input - switch between displaying and hiding the text input area, press and hold for input area menu (Palm keyboard or Graffiti area).


28.8.5. Application Help

Most Palm applications provide some level of on-screen help text. There is no standardised method of providing help screens. Some include help text directly within the operating screens, others provide a Help soft key or have Help (or Tips) within the menu options (see below). Others have an “i” symbol at the top of the screen which is pressed to bring up help,.

28.8.6. Menu Options


Each application has a set of drop-down menus that can be accessed from the Menu key on the Task Bar (see above) or by pressing the identifier tab at the top left hand side of the application screen.

The menu options vary depending upon the applications - example drop down menus for the Media application are shown below.

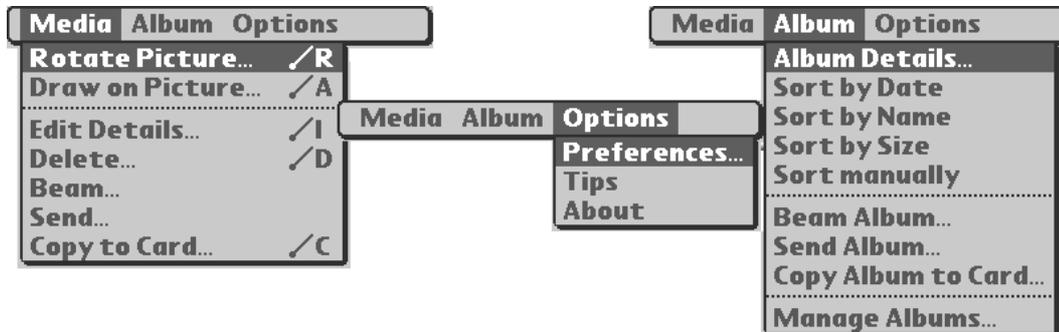

28.8.7. Categories

Most Palm applications include a drop-down menu at the top right of screen which is known as Categories. Initially this will be set to "All", but individual categories can be selected from the drop-down.

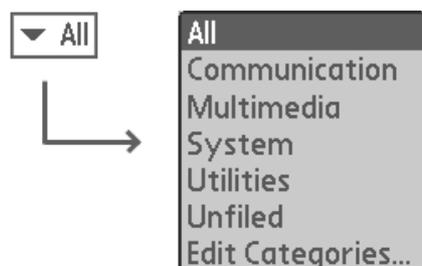

The concept of categories stems from the organisation of the Program Memory area of the device, see section [28.8.1](#). Most native Palm applications store both the program and the data for that application in the program memory area. This memory area does not have folder-based filing system. Categories can be regarded as Palm's folder system for the program memory area.

Each application (including the application called Applications) defines its own category list. Each category can be regarded as a sub-folder of the application. New categories can be created (and existing ones renamed or deleted) by selecting the Edit Categories function from the drop-down. One category which is always present and can not be deleted is Unfiled, this can be regarded as the root folder. Selecting "All" from the drop-down gives access to the contents of all of the categories including Unfiled.

NOTE The category list for the Media application is called Albums rather than Categories.

For basic applications, a document or file can be moved from one category to another by opening it in the application, changing the category setting, and then closing. More complex applications incorporate their own individual methods for moving data between categories.

28.8.8. Files and Folders on the Memory Card

Some applications, such as Media, Documents and pTunes, can operate with data that is stored both within the internal memory and on a memory card. Unlike the internal memory, the memory card will have a conventional folder structure and files can be directly copied to or from a PC.

Some applications define their own folder names for files on the card (DCIM in the case of Media, Documents in the case of Documents). Data stored from the Palm T|X onto a card, or transferred onto the card from a PC using Palm Desktop software will be automatically placed into the correct folder. However, files copied directly to the card must be manually placed into the correct folder.

Some other applications, such as pTunes, have a built-in folder browser and can access relevant files from anywhere on the card.

Categories

Applications such as Media and Documents retain the concept of categories for files on the memory card as well as files within the internal memory of the handheld.

The category list for the Media application is called Albums, and separate lists are maintained for the internal memory and the card. Creating a new album on the card creates a new sub-folder within the folder DCIM.

The category list for the Documents application combines all relevant files into a single list. An icon shows whether the document is on the card or within the internal memory of the handheld. Creating and changing categories does not affect the folder location. All files saved to the card as native Microsoft Office format will be in the folder Documents, while files saved in the alternative “native” format (e.g. Word to Go format) will be in the folder Palm/programs/DXTG. These latter files have the extension .pdb and can not be used on a PC except by using Palm Desktop software.

28.8.9. Communicating with Other Devices

Palm devices incorporate a variety of methods for communicating with peripherals, personal computers, and other handheld computers.

USB

All current Palm handheld computers incorporate a USB interface. This is intended for communication with a personal computer or another device that can act as a USB host (the handheld computer is defined as a USB peripheral).

- ! NOTE Do NOT try to make a direct USB connection to a PC which has not had the Palm software loaded onto it in advance. See section [28.3.1](#).

Serial

Some Palm handheld computers, including the Palm T|X, incorporate a UART based serial interface. This is used primarily for interfacing external peripherals such as keyboards. The PSA1301 uses this interface to communicate with the T|X.

Infra Red

Most handheld computers, including the Palm T|X, incorporate an infra red beam interface. This can be used to communicate with peripherals or laptop computers which have IR, but its primary purpose is to communicate with other handheld computers. The “Beam” command from the Palm menu system provides a quick and convenient way to transfer data (and even applications) to another handheld computer.

Bluetooth and WiFi

Many handheld computers, including the Palm T|X, now incorporate a Bluetooth wireless interface that allows them to communicate with other handheld computers, mobile phones, and personal computers. The Palm T|X also incorporate WiFi for wireless connection to a Network.

28.9. HotSync

HotSync® is the Palm method for “synchronising” data between the Palm T|X and a personal computer. Synchronising can encompass loading new files, updating (overwriting) existing files, and backing up files. The actions can be bi-directional. Exactly what is performed during a HotSync operation is defined within the Palm Desktop application on the PC. See Appendix B section [29.3](#).

HotSync requires that the standard Palm software applications are installed onto a personal computer. Users of the PSA1301T who do not intend to use Palm Desktop and other Palm PC applications should ignore HotSync.

28.10. Creating a Shortcut to PSAnalyzer

As supplied by TTI, the PSAnalyzer application is installed within the Palm TIX applications so as to occupy the first position within the Applications screen (category All or Unfiled). Other applications (apart from Quick Tour) are listed alphabetically.

It is easy to launch PSAnalyzer from the Applications screen either by pressing the icon directly, or by using the centre button of the 5-way navigator. However, it is also possible to change the settings of the TIX so as to be able to launch PSAnalyzer from a hard key or from Favourites.

Hard Key Shortcut

Open Preferences and select Buttons (under Personal). Choose a button (other than the Home button) and open the drop-down menu. Select PSAnalyzer and press Done.

Favourites Shortcut

Open the favourites screen and press the top left hand tab (which displays the time). Select Rearrange Favourites. Choose a favourite on Page 1 that is of low importance, highlight it and drag it firstly to the page 2 icon and then to an unused position on that page.

Select page 1, then press and hold the newly created unused position - the Edit Favourite dialogue box will appear. Set Type: App, Original: PSAnalyzer (from drop-down), Name: PSAnalyzer. Press OK. Select and drag to the desired position on page 1. Press Done.

28.11. Additional Software Applications

A very large number of additional software applications are available for the Palm handheld computer. Some come directly from Palm, but the larger number come from third party sources.

Note: TTI does not promote, endorse or provide support for any applications. The following information is provided for guidance only.

Most applications are commercial with typical prices between US\$10 and US\$50, though some are free of charge. Most applications can be "tried" before purchase. There are three main ways to find software applications:

Addit

Addit is pre-installed onto the Palm TIX. Its primary purpose is to provide a conduit for buying additional software applications. It also offers access to News and to Tips & Tricks.

Addit requires Palm desktop software to be installed onto your PC. The new applications (or News items and Tips & Tricks) are downloaded to the PC and transferred to the handheld during a HotSync operation.

The Palm website

Palm websites are country specific, but can be accessed through the route address of **www.palm.com**. A link can then be found to Software, from which a wide range of software applications can be purchased, normally priced in local currency.

Third Party websites

There are many third part websites that provide access to fully commercial software, shareware, or freeware. These can be found by using a Search Engine. Useful search phrases may be Palm Software, Palm Applications, PDA Software, Handheld Software, etc.

28.11.1. Installing additional applications without using Palm Desktop

Where the user has installed Palm Desktop software onto their PC, this should be used to install new applications. The sub-application Quick Install is provided for this purpose. However, it is also possible to install some software application using the memory card and card reader, see section [23.3.1](#).

Note: Only applications which consist of a single .prc file can be installed in this way. Applications which include an additional file such as a .pdb file, must be installed using Palm Desktop or Quick Install.

Software applications are normally installed in the main memory of the handheld. Some applications can be run directly from the memory card, but others have to be installed in the main memory by copying them from the card.

Having downloaded (or otherwise copied) a software application to a PC, use the card reader to copy the program file (which will have the extension .prc) to the card. The file must be copied to the directory \Palm\Launcher.

When the card is inserted back into the Palm T|X, the Applications screen is automatically switched to show the applications which are on the card. (To return to the normal Applications screen, select the drop down menu at the top right and select "All" in place of "Card").

To copy a program from the card to the main memory, select Menu Options by pressing the time display at the top LH side of the Application screen, then select Copy. Change the "Copy from" drop down from Device to Card, then select the required program from the list and press Copy.

29. Appendix B. Palm Desktop Software

The following information is provided as guidance for PSA1301T users.

See the Palm documentation for details of how to use Palm Desktop.

29.1. Deciding whether to install Palm Desktop

The documentation provided by Palm with the T|X instructs the user to install the Palm Desktop software immediately. TTI advises users of the PSA1301T to consider their particular circumstances before deciding whether to install it (and where to install it).

Palm Desktop is NOT needed for any of the functions of PSAnalyzer on the PSA1301T.

However, if it is intended to use the Palm T|X as a personal organizer, Palm Desktop may be very valuable. It also provides a convenient means of converting Microsoft Office documents, and for loading new applications and backing up data.

29.2. The purpose of Palm Desktop software

Palm Desktop is the companion software application for linking the Palm T|X (or other Palm handheld computers) to a PC. It is a powerful piece of software which enables the user to maintain data simultaneously on the handheld computer and on the PC.

Palm Desktop can be installed in any of six languages: English, Deutsch, Français, Español, Italiano, or Português.

Palm Desktop includes modules for managing Calendar, Contacts, Tasks, Memos, Expense, Note Pad, Media, Documents, and VersaMail. The "Documents" module (Documents to Go) is actually a stand-alone module which has the function of converting and transferring Microsoft Office files (Word, Excel and Powerpoint).

29.3. HotSync

The key to Palm Desktop is HotSync. HotSync transfers data between the two devices so as to maintain them in synchronism. So, for example, when a new contact name is added to the contacts list on either device, performing a HotSync operation automatically updates the other device.

HotSync also provides an automatic backup onto the PC both of data, and of programs which are not within the ROM of the Palm T|X. HotSync is normally performed using a USB connection, though it can also be done via a modem or over a network using a wireless connection.

The USB cable supplied by Palm with the Palm T|X includes a button which automatically initiates HotSync. However, it can also be initiated from the HotSync icon on the Applications screen. This method should be used when the Palm T|X is fitted into the PSA1301T.

29.4. Palm T|X User Name

Palm Desktop creates a "pairing" relationship between a PC and a Palm T|X. It creates a User Name for the Palm T|X which is written into the device firmware and can not subsequently be changed (other than by a hard reset). The User Name must be unique as it identifies a particular device and ensures that if another device is connected to the PC, files will not be accidentally overwritten by a HotSync operation.

The user name can be seen at the top right of the screen by selecting the HotSync application. The Palm T|X supplied with the PSA1301T does not yet have a user name.

A user name is only required if Palm Desktop software is to be used. The user name is created when the first HotSync operation is done.

29.5. Palm Desktop software and Windows PCs

Palm states that for a full installation including Palm Desktop software, the PC must be running Windows 2000 or Windows XP and that admin rights will be required to install. One available USB port is needed. Other operating systems that support USB may be useable, but functionality will be reduced.

Palm Desktop includes modules for managing Calendar, Contacts, Tasks, Memos, Expense, Note Pad, Media, Documents, Quick Install and VersaMail. Quick install is a stand-alone module for installing new applications and files onto the handheld. A background program called HotSync manager is also installed.

29.6. Palm Desktop software and Apple Macintosh computers

Palm states that for a full installation including Palm Desktop software, the Mac must be running OS 10.2.6 or above and that admin rights will be required to install. One available USB port is needed.

The full installation of Palm Desktop includes modules for managing Calendar, Contacts, Tasks, Memos, Expense, Note Pad, Media, Documents, and VersaMail. There is also a Send to Handheld droplet for installing new applications and files.

29.7. Installation Procedure

Palm Desktop is a substantial suite of software for installation onto a PC (Windows or Mac). The installation procedure takes some time, and may require a reboot (depending upon the operating system). Inserting the CD should cause the installation to start automatically.

Once the software is installed, a screen appears showing the current step in the procedure i.e.

1. Install software > **2. Synchronise device** 3. Register device 4. Install extra software

On pressing Continue, a dialogue box appears for "Enter Your User Name". This step can not be skipped. This user name will be allocated to the Palm T|X at the next stage. The name must be unique, if another Palm handheld device (that might be seen by this computer) had the same user name problems could occur.

After entering a user name, the next screen provides a choice of Synchronise with Palm Desktop or with Microsoft Outlook. This choice can be changed later from within Palm Desktop.

The next screen instructs you to "Sync your Device and Computer". There are two options: initiate a HotSync or Skip. What happens next depends upon which you choose.

Either: Initiate HotSync

The screen instructs you "press the HotSync button" on the USB cable to begin. If the Palm T|X is mounted within the PSA1301T, it will be connected via the mini USB cable and there will be no HotSync button. In this case, select HotSync from the applications screen and press the HotSync symbol on the screen.

HotSync commences using the default settings of Palm Desktop to synchronise and backup files. This may take several minutes. The User Name entered earlier in the set-up is written to the firmware of the Palm T|X.

Or: Skip

The screen warns that "unexpected results can occur". No HotSync takes place, no files are transferred, and no User Name is transferred.

The installation then progresses to the "Register Device" stage, and finally to the "Discover your Device" screen which provides the option of adding extra software.

Note: Once Palm Desktop has been installed on a PC, the "Discover your Device" screen can be returned to at any time by re-inserting the CD.

29.8. Using multiple devices with one PC, or a device with multiple PCs

An instrument such as a PSA1301T is likely to have a different usage pattern from a stand alone handheld computer. One department may have several devices and may wish to use them with more than one PC which has Palm Desktop installed.

Palm Desktop caters for this by maintaining separate accounts and folders for different "users" (i.e. devices with different user names). Each user can have its own custom HotSync settings which defines exactly what happens when a HotSync takes place on that PC.

When a HotSync is initiated on a device which has a user name that Palm Desktop does not recognise, it asks if new user account should be created. On confirmation, HotSync continues using default HotSync settings.

When a HotSync is initiated on a device which does not yet have a user name, a dialogue box appears prompting to select an existing user name, or enter a new user name. That user name is then written to the firmware of the Palm T|X and HotSync continues.

Note that a new user can be set up within Palm Desktop prior to the relevant device being connected (select Edit Users from the drop down at the top right). This has the advantage that custom HotSync settings can be defined prior to the first HotSync being initiated. For example, all actions could be set to "do nothing" except for Backup.

29.9. HotSync transfer of PSAnalyzer Screen Images to a PC

Palm Desktop has no conduits for PSAnalyzer files and therefore can not be used for the general transfer of PSAnalyzer files. However, screen images are recognised by the Media application and are therefore transferred to a PC when a HotSync operation is performed (provided that the custom HotSync action for Media remains suitably set within Palm Desktop).

The folder location on a Windows PC will be as follows:

```
C:\Program Files\Palm\ "user-name" \Photos\offline copy location\ "nnnn" \PSAnalyzer
```

Where "user-name" is the Palm T|X User Name (see section [29.4](#)) and "nnnn" is a four digit hex number assigned by Palm Desktop to the memory card.



Thurlby Thandar Instruments Ltd
Glebe Road, Huntingdon, Cambridgeshire PE29 7DR, England
Telephone: 44 (0)1480 412451 Fax: 44 (0)1480 450409
e mail: sales@tti-test.com
International website: www.tti-test.com UK website: www.tti.co.uk

Book Part No. 48511-0870 Issue 2