

1. Introduction.....	2
Features.....	2
Intended use.....	2
Using this manual.....	2
Symbols.....	2
2. Getting started.....	3
File.....	3
Connect.....	3
Help.....	3
Instrument control panel.....	4
3. Instrument setup.....	5
Select an instrument.....	5
4. Instrument control.....	6
5. Selecting a channel.....	6
Turning channels on and off.....	6
Setting a value.....	7
Settings menu.....	7
6. Logging.....	7
Overview.....	7
Logging setup.....	8
Logging controls.....	8
Recording channel setup.....	9
View.....	10
7. Sequencing.....	11
Overview.....	11
Sequencing setup.....	11
Saving/ loading a sequence.....	13
Running a sequence.....	13
8. Error log and Communications.....	14
Error log -A.....	14
Communications -B.....	14

1. INTRODUCTION

Features

Multi Instrument Control

Logging to table and graph format

Timed sequence control across all instruments and channels

USB, LAN and RS232 compatible

Intended use

List of compatible instruments:

POWER SUPPLIES		LOADS	
Series	Models	Series	Models
CPX	CPX200DP, CPX400DP, CPX400SP	LD	LD400P
MX	MX100TP, MX100QP, MX180TP	LDH	LDH400P
PL	PL-P & PLH-P		
QL	QL-P Series I & II		
QPX	QPX1200SP, QPX600DP, QPX750SP		
TSX	TSX-P Series I & II		

Using this manual

Colour coding:

Green = Larger view of a selected area

① Orange = Instruction to select

① Blue = Optional instruction to select

① Yellow = Description of item

Symbols

The following symbols are displayed throughout the manual:

CAUTION



Indicates a hazard that could damage the product that may result in loss of important data or invalidation of the warranty.

NOTE



Indicates a helpful tip

2. GETTING STARTED

File


Open / Save Configuration Open or save the instrument control and recording channel configurations.

Exit - Close the application.



Connect

Add Network Instrument- Specify the IP address or host name and enter the port number (generally 9221 or 5025) – see the instrument's Instruction Manual for more details. Click the **PING** button to test the connection- if successful the **USE** button will activate. Click the **USE** button to continue.

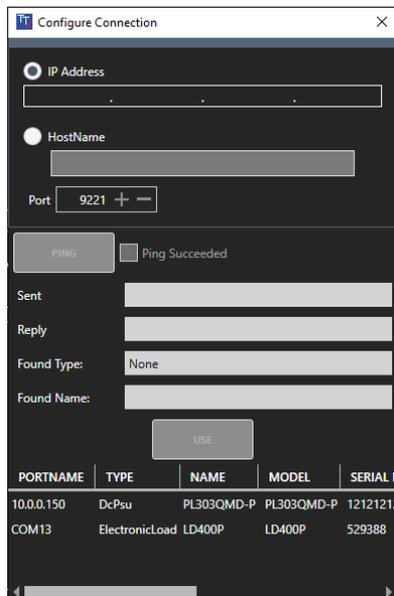

Check Local Ports (USB & RS232)- Refreshes the list of available instruments.

NOTE



Following a power cycle, checking ports can take up to 10 seconds if not connected via LAN.

Help

Help - PDF guide to using the software.

About- Application details and a 'report generator' function to provide feedback.

Instrument Control Panel

The Instrument Control Panel is selected using the icon ①

Up to four instruments can be connected to the Control Panel. Each instrument will populate one control box ②.

For details on how to use the instrument control box, see **Error! Reference source not found..**

3. INSTRUMENT SETUP

Select an instrument

Firstly, ensure Instrument control is selected ①.



Select the drop-down box in the Instrument control window ② to show all instruments available.

If a connected instrument is not shown, refer to Connect.

The available instruments will be listed under the instrument name e.g 'MX100QP' for the MX100QP Quad Output Multi-Range DC Power Supply.

Select the instrument ⑧ to activate the instrument control.

The instrument name will now be shown ③, in addition to the COM port details or IP address ⑤ in the top of the instrument control box. There will also be allocated a coloured strip ④ on the left, indicating the product category.

The instrument can be given a unique name, using the edit box ⑥.

The meter digits show live readings when the channel is on, and the digits will be shown in yellow (CH1). If the output is off, the displayed digits show the set values, and are shown in grey.

NOTE



The channel output state will match the instrument when connected, this may be on or off depending on the setup.


To disconnect an instrument, select the connected instrument from the drop-down box. This will reset the control box back to the default state. If an instrument is connected and communication is lost, a 'Comms Error' will show ⑦. Check connections and reconnect as shown above.

NOTE



It is recommended that instruments are disconnected before powering down.

4. INSTRUMENT CONTROL

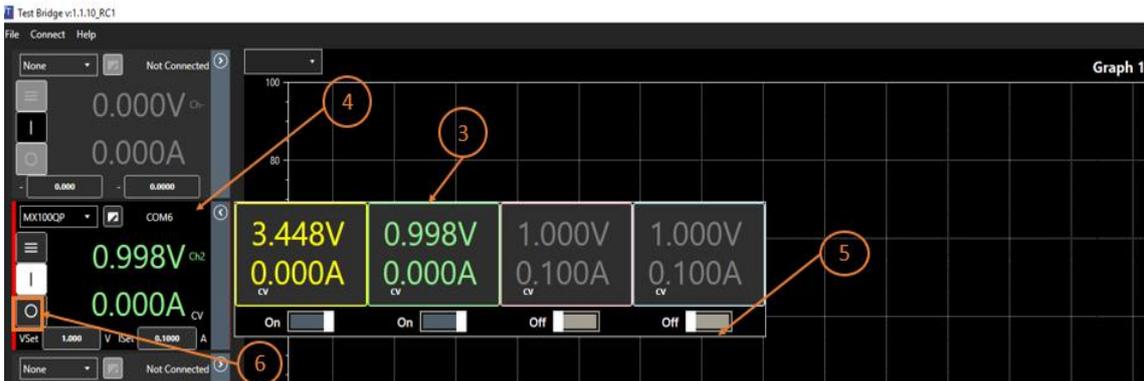

Selecting a channel

(Multi - Channel Instruments)

The Instrument Control Box ① displays and setting of the active channel, The active channel number ② will match the selected channel colour. The meter will show Channel 1 when first activated.

To select a different channel, first select > to display all available channels . The channel numbers run in ascending order and start at 1 closest to the Instrument Control Panel. Each channel is shown in a different colour The channel control can be active or hidden at any time using the < and > buttons.

Select the active channel by clicking on the channel meter ③ - this will then change the main instrument control ④ to reflect the readings and settings for that channel.

Turning channels on and off

Single Channel

To turn the channel output on or off, use the ON/OFF toggle ⑤ below the channel.

When the channel is on, the meters on the control box show the live data for each available channel, when the output is off the meter shows the set values for each channel (grey).

Multi Channels (All On/All Off)


It is possible to turn all the channels on or off simultaneously with the All ON or All OFF ⑥ buttons on the Instrument Control.

NOTE



The Multi-Channel control box does not need to be shown to use the All ON or All OFF buttons.

Setting a value

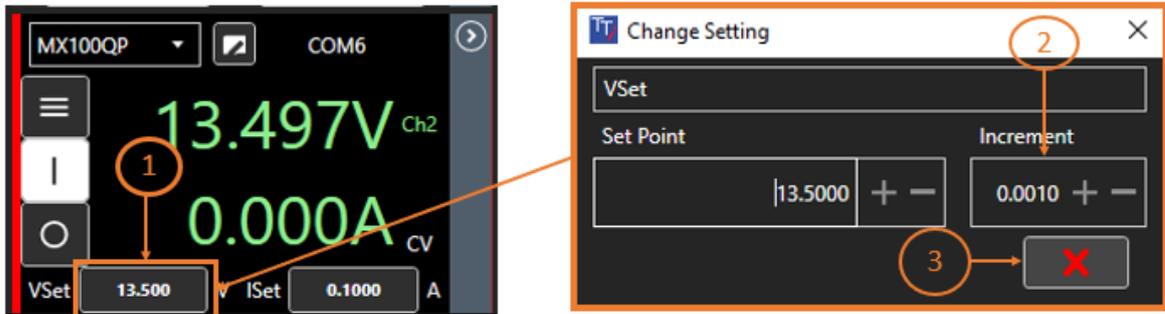

The active channel settings are changed using the “VSet” and “ISet” settings fields ①. These show the set values. For electronic load “VSet” and “ISet” will be replaced by “Level A” and “Level B”.


To change the value, select the field. A pop-up will appear with the setting options.

Values can be entered by selecting and editing, either by using the keyboard or the mouse wheel to increase/decrease the value.

These changes will show on the instrument as they are changed in the Change Setting pop-up.

Close the Change Settings pop-up using the X button ③.

Settings Menu

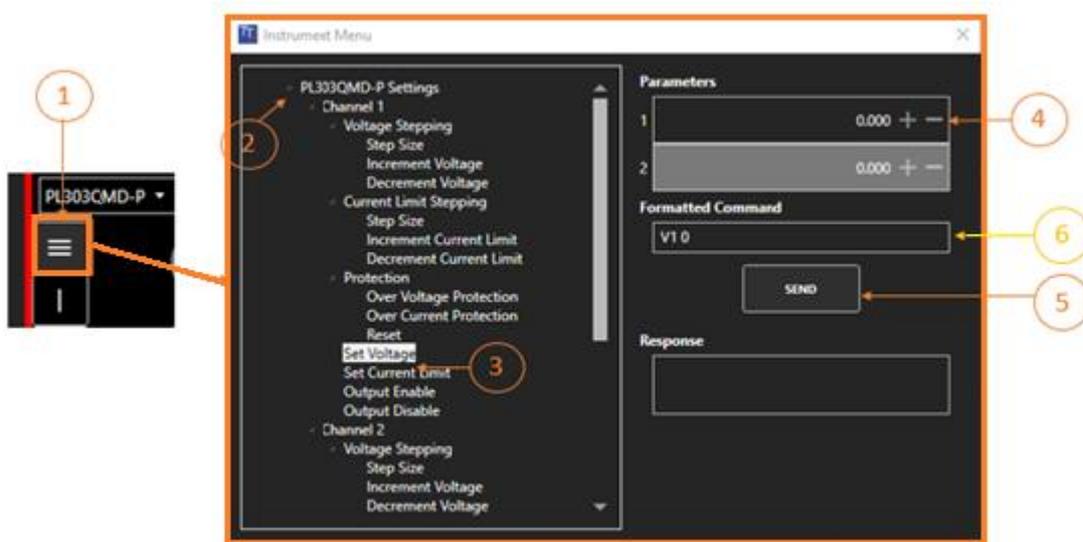

To access the instrument settings, select the Settings Menu button ①.

This menu contains settings and functions such as OVP, limits, ranges etc. These are instrument specific and will vary depending on the instrument connected.

Each block of settings is contained within a tree view ②, the selected setting on the left ③ defines the available parameters ④ on the right. If no parameter is available, the action has no numeric value option.

Press SEND ⑤ to send the formatted command ⑥.


5. LOGGING

Overview

Logging uses recording channels to capture live data; channels can be set to record values from any channel on an active instrument at specified time intervals. A maximum of 8 parameters can be logged from any active channel. Varying measurement intervals can be set alongside units and plot line colour. The results are plotted on one of the two available graphs and can also be viewed in a

table and exported as a .CSV (comma separated values), a .TSV file (tab separated values) or as a plain text file. The graph provides advanced zooming and panning functions, allowing for efficient data analysis.

Logging setup

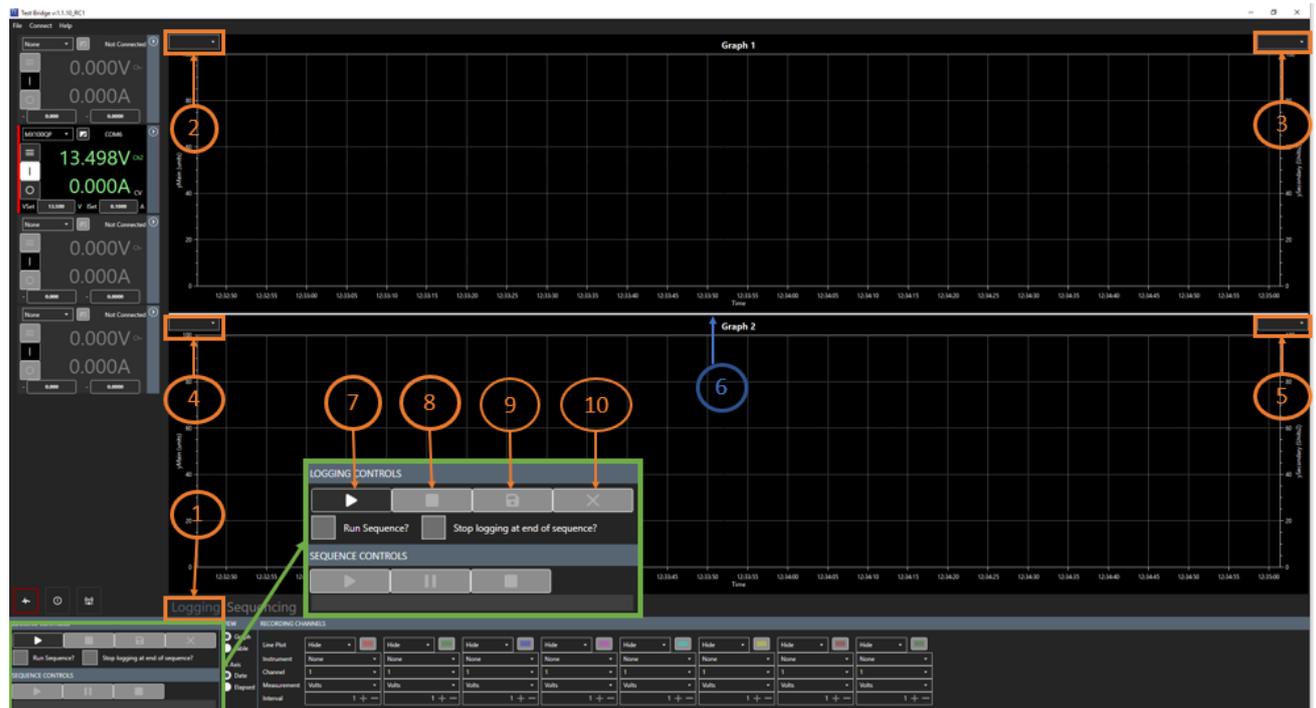

Firstly, select logging mode ①. Before starting, select the primary and secondary units to record on the Y axis using the drop-down boxes on either side:

Graph 1= ②, ③

Graph 2= ④, ⑤

The X axis will always show time (absolute or relative).

The bar ⑥ can be used to change the proportion of each graph shown.

Logging controls

Once the recording channels have been setup, data logging is controlled using the logging controls:

Run - ⑦ Start logging selected data

Stop - ⑧ Stop logging selected data

Save- ⑨ Save the logged data as a file (CSV, TXT or TSV)

Clear-⑩ Clear all logged data.

NOTE



'Save' will only save the logged data. To save instrument setups, see File, tools, help.

TSV - Tab Separated Variable


CSV - Comma Separated Variable

CAUTION



The 'Clear' action is irreversible. Save any important data before clearing.

Recording channel setup

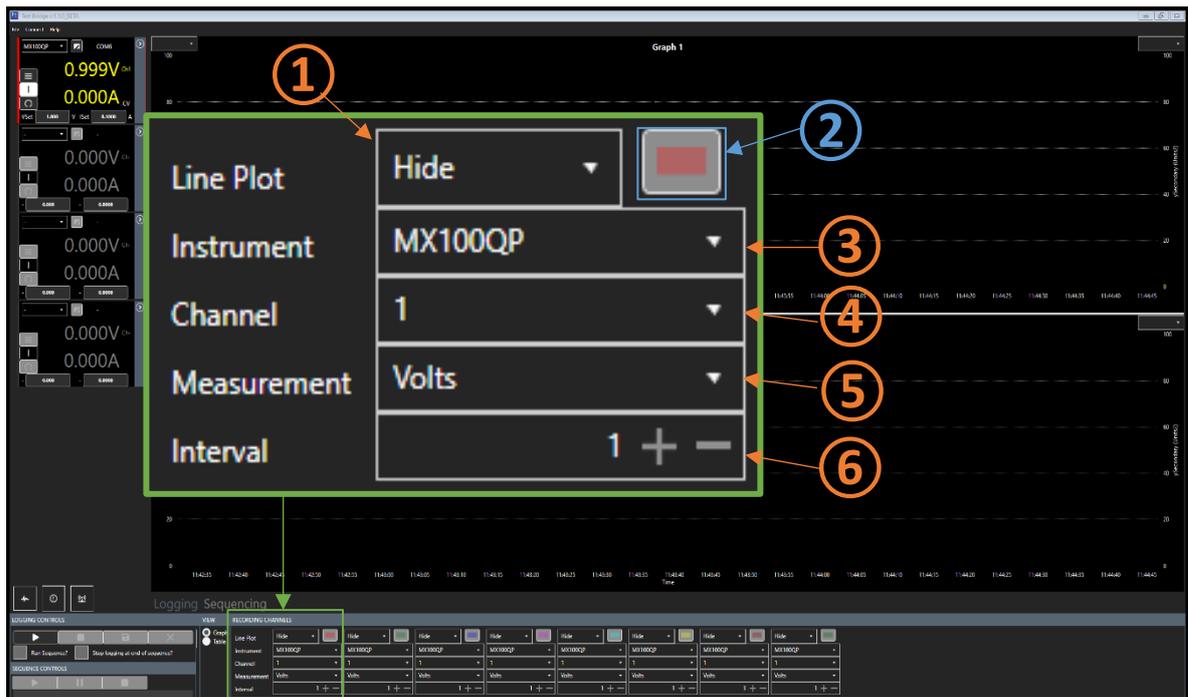

NOTE



Ensure Y axis units have been set before setting recording channels, see [Logging setup](#) for more details.

Line plot - Select the preferred graph ① to show the logged data on using the drop-down box. This can also be set to hide; the data will not be shown on the graph but will still be logged. The colour of the logging line can be selected from the colour picker ②.


Instrument - Choose which instrument ③ to log the data from using the drop-down box. Only instruments that have been allocated a control panel will be available in the drop down.

Channel - Select the channel ④ to log data from the chosen instrument.

Measurement - Select the measurement units ⑤ to be logged. Ensure the units match the units set on the graph.

Interval - Set the logging interval ⑥ in seconds, the minimum is 250ms. To ensure the best results, check the minimum sampling rate specifications in the instrument's Instruction Manual.

View

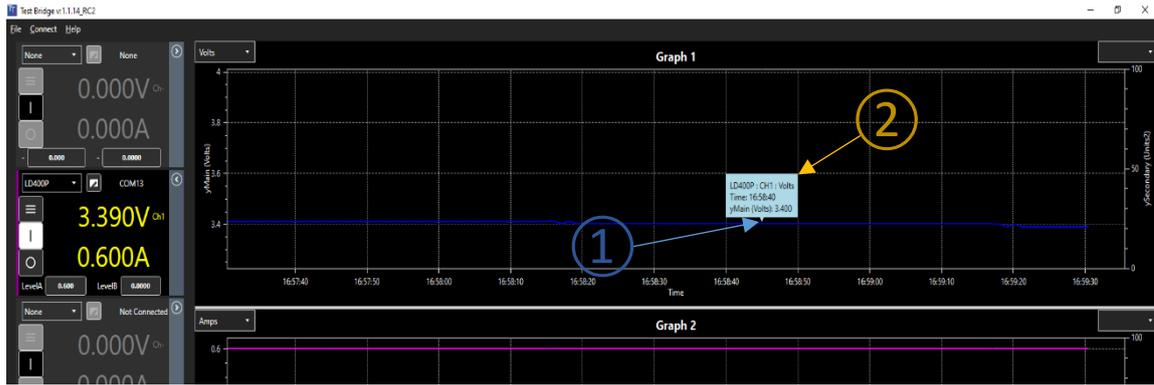

When the data is recorded and displayed on a graph, it can be viewed in several different ways:

Show values - Click and drag the mouse across the graph **1** to show the details **2** of that specific point in the logged data. This can be dragged along the entire data line to show any point within the log. The following actions are available for graph navigation. To begin, click on the graph area:

 Pan	Right click and drag	Alt + left click and drag	Arrow keys	 fine pan	Ctrl + Right click and drag	Ctrl + Alt + left click and drag	Ctrl + Arrow keys
 Zoom	Mouse wheel (if available)	Numeric keypad +/-	Page Up / Page Down	 Fine zoom	Ctrl + mouse wheel	Ctrl + numeric keypad +/-	Ctrl + Page Up / Page down
 Zoom a rectangle	Ctrl + right-click and drag	Middle mouse button	Ctrl + Alt + left click and drag	 Reset zoom	A on the keyboard,	Right click select Reset Zoom	Alt + Ctrl + left double click

Note: To zoom in one axis only, place the cursor over the axis, then use the mouse wheel to zoom

TIMESTAMP	ELAPSED	LOG#
02/08/21-13-134720	0000:0000	0.739
02/08/21-13-134825	0000:0104	6.237
02/08/21-13-134843	0000:0223	8.803
02/08/21-13-135055	0000:0334	5.001
02/08/21-13-135168	0000:0447	0.999
02/08/21-13-135277	0000:0557	3.764
02/08/21-13-135360	0000:0669	8.802
02/08/21-13-135513	0000:0792	7.511
02/08/21-13-135639	0000:0918	1.764
02/08/21-13-135765	0000:1044	2.649
02/08/21-13-135869	0000:1148	8.236
02/08/21-13-135975	0000:1255	8.235
02/08/21-13-140083	0000:1362	2.649
02/08/21-13-140197	0000:1476	1.196
02/08/21-13-140299	0000:1578	5.002
02/08/21-13-140409	0000:1688	8.802
02/08/21-13-140517	0000:1796	6.237
02/08/21-13-140630	0000:1909	1.764
02/08/21-13-140741	0000:2020	2.649

Table

Any logged data can also be viewed in a tabular format. To change the view, select **Table 4**.


The data is arranged in columns. Each active recording channel is allocated a LOG number, ascending from left to right- 1 to 8.

6. SEQUENCING

Overview

Sequence numbers are limited only by the number of channels that are available; each sequence is allocated to a specified channel on an instrument. Two different parameters can be added to each sequence, along with two events. A range of built-in step options are available, including: sine wave, triangle wave, ramp, and step.

Sequencing setup

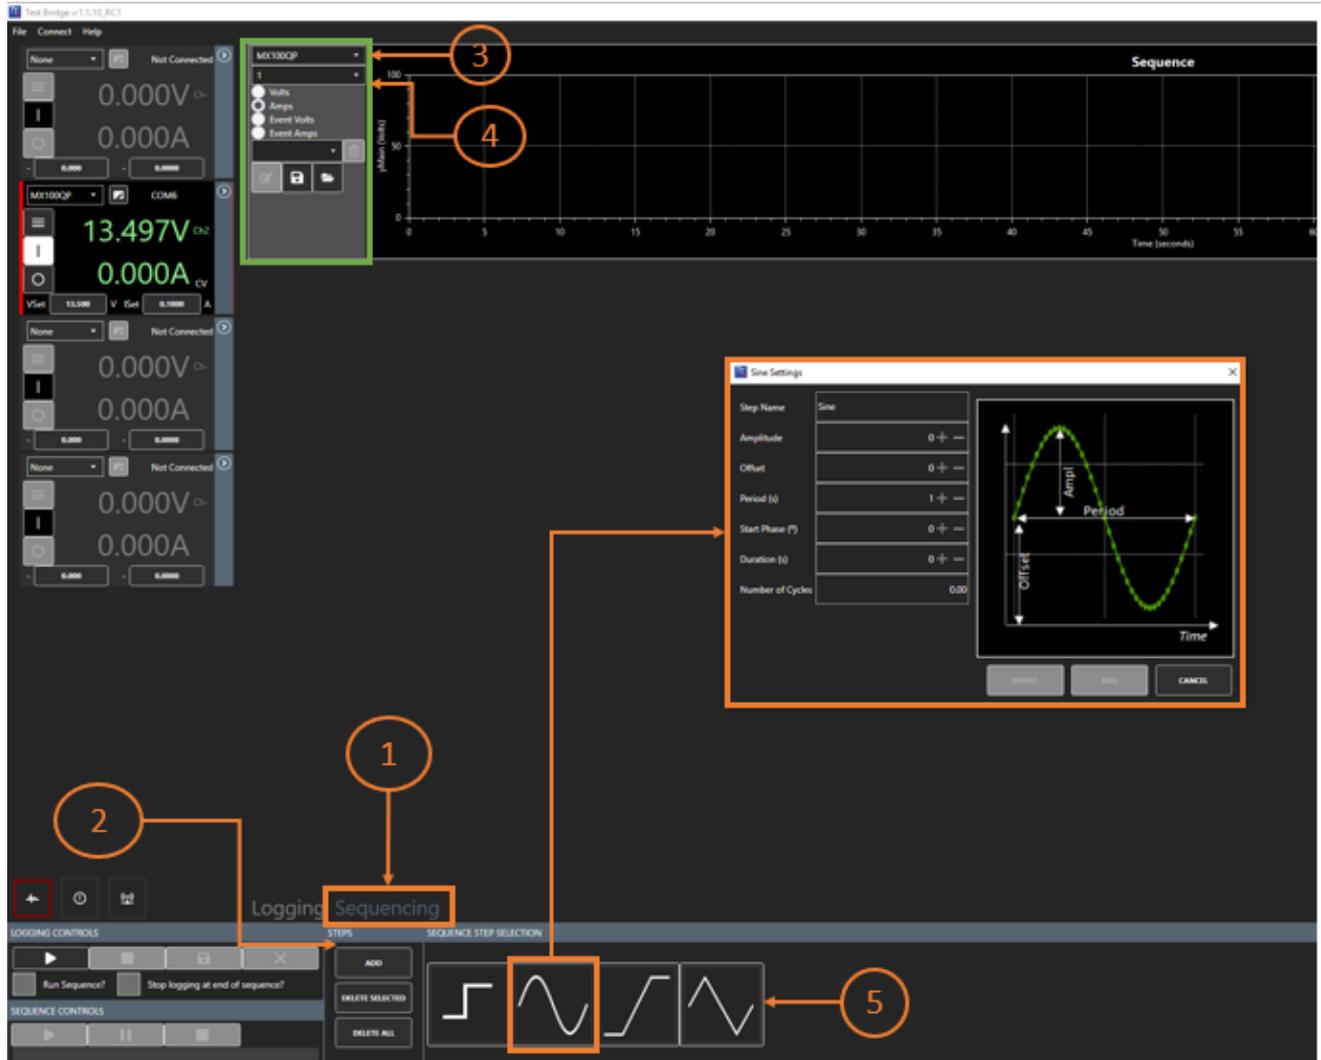

Firstly, select Sequencing mode ①, then select **Add** ② to start creating a sequence.

Each sequence is allocated to a specified channel. Before the sequence can be created, an instrument ③ and channel ④ need to be specified. Use the drop-down boxes to select these. The sequencing tools will now be available to use.

NOTE



The sequence update period is limited to 250ms. Dots represent the update points, with linear lines joining points. i.e. A sine wave set for 1s period will have 5 points and be represented as a triangle.

Adding steps to a sequence

Each individual channel sequence can contain a primary and secondary parameter, and an event for each parameter. These are selected using the radio buttons and colour coded for identification.

To add a step to the sequence, select the parameter or event, then select a shape from the four options in the step selection (5). Each shape has a unique pop-up window that gives the editable parameters for that shape:

Each step has the option to Insert, Add or Cancel:

INSERT- Place the step BEFORE the selected step.

ADD- Place the step AFTER the last step.

CANCEL- Return to the sequence without making any changes.

There is also an option to name the step.

When creating a step for an event, additional options are available to add a condition and an action.


Editing a sequence

NOTE



When steps are added to the sequence, they are controlled by the sequence control and can be edited by selecting Step (1) and clicking Edit option (3).

Steps that have been added to the sequence can be selected using the drop-down box (1). The steps are highlighted in the sequence with a faint box the same colour as the unit/event.

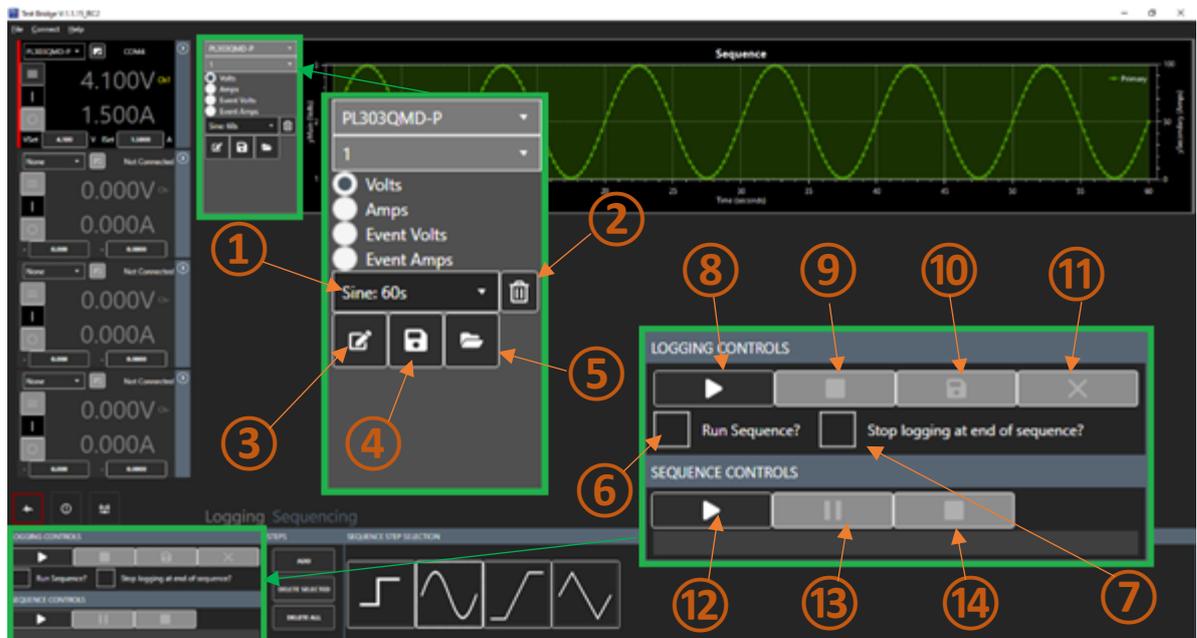

(1) - Step selection drop down

(2) - Deletes the current step

(3) - Edits the sequence step selected in (1)

(4) - Saves a sequence file

(5) - Opens a sequence file

(6) - When ticked causes the sequence to start when logging starts

(7) - When ticked logging will stop when the sequence stops

(8) - Starts logging data, if (6) is ticked the sequence will also start

(9) - Stops logging data, if (6) is ticked the sequence will also stop

(10) - Saves log data to file

(11) - Clears all log data

(12) - Start/continue the sequence

(13) - Pause the sequence

(14) - Stop the sequence

Steps can be deleted once they are selected using the trash can (2).

Steps can be edited once they are selected using the edit button (3).

Saving/ loading a sequence

Sequences can be saved using the **Save** button ④ and loaded using the **Load** button ⑤.

NOTE



'Save' will only save the sequence settings. To save instrument setups, see File> Tools>Help.

'Load' will load steps for all units, not just the selected unit.

Running a sequence while logging

Once the sequence setup is complete, it can be run by selecting Run Sequence ⑥, followed by the Run button ⑧ on the logging controls.

The logging graph will then show the logging results for the running sequence, provided the recording channels have been set to view the channel allocated to the sequence. See Recording channel setup for more details.

⑧ will start logging and run the sequence if ⑤ is ticked.

⑬ - Pause the sequence

⑭ - Stop the sequence

Running a sequence independently of logging

Once the sequence setup is complete, it can be run by selecting ⑫. ⑥ must be un-ticked to be able to run a sequence independently of logging.


⑫ - Start/continue the sequence

⑬ - Pause the sequence

⑭ - Stop the sequence

7. ERROR LOG AND COMMUNICATIONS

Error log - A

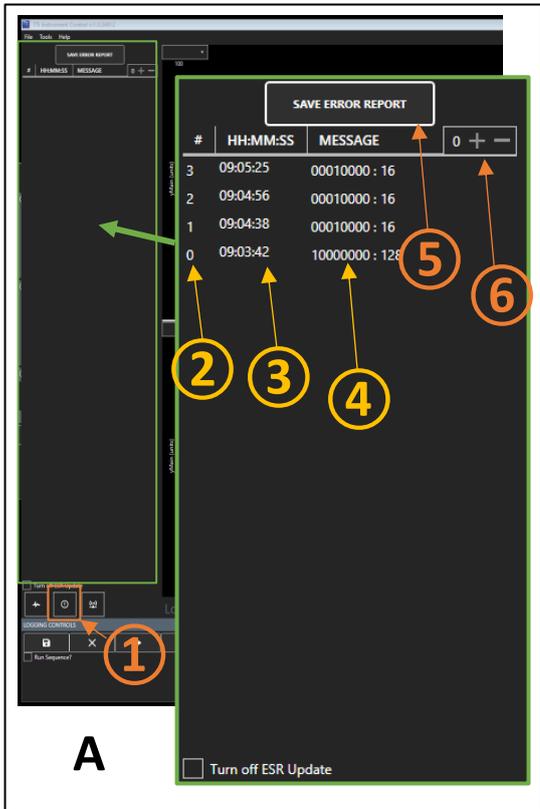


The Error Log panel is selected using the icon ① and will present any errors that have been logged.

Each error message ④ has an index number ② and time allocated ③ as a reference point.

The Error Log can be saved using the Save Error Report button ⑤.

To change the instrument, select the number reference ⑥ using the +/- keys. Numbers run from 0-3 starting with the first instrument at 0.

Communications - B

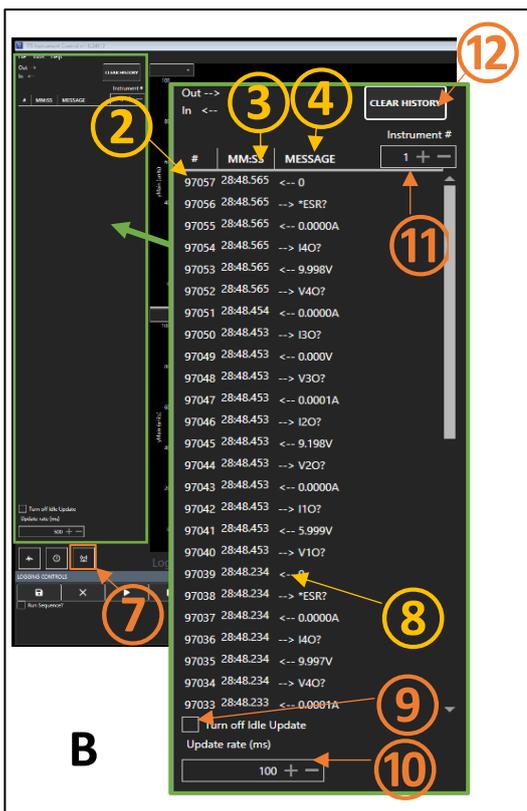

The communications panel is selected using the icon ⑦.

The communications panel shows the commands used to communicate between Test Bridge and the connected instruments.

Messages ④ are either a sent or received command this is indicated with the Out/In arrows ⑧. Each message has an index number ② and time allocated ③ as a reference point.

To change the instrument, select the number reference ⑪ using the +/- keys. Numbers run from 0-3 starting with the first instrument at 0.

Messages are recorded at the selected interval update rate ⑩ - the minimum is 100ms. Messages are recorded even when the instrument is idle. To stop communications recording idle data, select the Turn Off Idle update ⑨.

The history can be cleared using the clear history button ⑫.